

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072118\
 Data File : VU025583.D
 Acq On : 21 Jul 2018 14:26
 Operator : MD/SY
 Sample : J4039-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.670	23	25	27	rBV2	209	78	0.01%	0.001%
2	0.706	33	36	39	rBV	357	188	0.02%	0.002%
3	0.751	47	50	51	rBV	129	77	0.01%	0.001%
4	0.818	67	71	73	rBV2	297	223	0.02%	0.002%
5	0.851	78	81	84	rBV	267	167	0.02%	0.002%
6	0.944	107	110	113	rVB2	256	163	0.02%	0.002%
7	0.957	113	114	117	rVB	94	42	0.00%	0.000%
8	0.986	117	123	126	rBV2	296	347	0.03%	0.004%
9	1.092	139	156	175	rBV	447541	518019	49.03%	5.562%
10	1.404	246	253	266	rBV	117911	122463	11.59%	1.315%
11	1.687	333	341	361	rVB	96119	122066	11.55%	1.311%
12	2.278	515	525	537	rVB	216243	327815	31.03%	3.520%
13	2.722	661	663	669	rBV2	446	393	0.04%	0.004%
14	2.841	699	700	703	rBV	316	97	0.01%	0.001%
15	2.953	732	735	736	rBV	281	170	0.02%	0.002%
16	3.088	774	777	780	rVB	420	250	0.02%	0.003%
17	3.108	780	783	784	rBV	560	281	0.03%	0.003%
18	3.159	797	799	800	rBV	141	60	0.01%	0.001%
19	3.201	809	812	813	rBV	214	104	0.01%	0.001%
20	3.272	829	834	838	rBV2	285	335	0.03%	0.004%
21	3.304	842	844	846	rBV2	473	290	0.03%	0.003%
22	3.349	856	858	862	rVB2	258	134	0.01%	0.001%
23	3.371	862	865	868	rBV	279	167	0.02%	0.002%
24	3.429	877	883	885	rBV2	344	317	0.03%	0.003%
25	3.461	891	893	897	rVB2	368	198	0.02%	0.002%
26	3.494	897	903	905	rBV2	163	204	0.02%	0.002%
27	3.548	917	920	923	rBV	320	180	0.02%	0.002%
28	3.571	923	927	929	rVB	213	165	0.02%	0.002%
29	3.587	929	932	936	rBV	350	209	0.02%	0.002%
30	3.609	936	939	940	rBV2	172	91	0.01%	0.001%
31	3.648	949	951	956	rBV2	154	126	0.01%	0.001%
32	3.744	978	981	983	rBV2	418	265	0.03%	0.003%
33	3.802	994	999	1002	rVB2	187	174	0.02%	0.002%
34	3.821	1003	1005	1008	rBV2	221	122	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072118\
 Data File : VU025583.D
 Acq On : 21 Jul 2018 14:26
 Operator : MD/SY
 Sample : J4039-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	3.892	1025	1027	1028	rBV2	148	64	0.01%	0.001%
36	3.950	1038	1045	1046	rBV	353	340	0.03%	0.004%
37	4.056	1075	1078	1082	rBV2	176	100	0.01%	0.001%
38	4.072	1082	1083	1085	rVB	179	49	0.00%	0.001%
39	4.114	1092	1096	1097	rBV	381	255	0.02%	0.003%
40	4.178	1102	1116	1145	rVV	84481	215566	20.40%	2.315%
41	4.590	1242	1244	1246	rBV	253	129	0.01%	0.001%
42	4.654	1246	1264	1284	rVV	181680	425119	40.24%	4.565%
43	4.860	1322	1328	1330	rBV	298	303	0.03%	0.003%
44	4.879	1330	1334	1336	rBV2	954	671	0.06%	0.007%
45	4.934	1349	1351	1354	rBV	141	91	0.01%	0.001%
46	4.989	1365	1368	1374	rVB3	651	668	0.06%	0.007%
47	5.053	1386	1388	1394	rVB2	354	277	0.03%	0.003%
48	5.079	1394	1396	1397	rBV2	178	57	0.01%	0.001%
49	5.092	1397	1400	1403	rVV2	183	135	0.01%	0.001%
50	5.165	1421	1423	1424	rBV	179	70	0.01%	0.001%
51	5.175	1424	1426	1427	rBV	194	80	0.01%	0.001%
52	5.346	1453	1479	1506	rBV2	355634	1056463	100.00%	11.344%
53	5.625	1564	1566	1569	rBV2	252	212	0.02%	0.002%
54	5.667	1576	1579	1580	rBV2	259	122	0.01%	0.001%
55	5.735	1597	1600	1601	rBV	389	182	0.02%	0.002%
56	5.805	1621	1622	1624	rBV	172	77	0.01%	0.001%
57	5.892	1632	1649	1670	rBV	429455	833986	78.94%	8.955%
58	6.175	1735	1737	1739	rVB	462	192	0.02%	0.002%
59	6.188	1739	1741	1743	rBV	381	208	0.02%	0.002%
60	6.259	1757	1763	1764	rBV2	271	269	0.03%	0.003%
61	6.336	1773	1787	1815	rBV	244335	483829	45.80%	5.195%
62	6.522	1842	1845	1847	rBV2	207	85	0.01%	0.001%
63	6.564	1855	1858	1860	rBV3	392	237	0.02%	0.003%
64	6.616	1867	1874	1884	rBV7	1553	2980	0.28%	0.032%
65	6.664	1887	1889	1891	rVB2	135	50	0.00%	0.001%
66	6.686	1891	1896	1898	rBV2	290	279	0.03%	0.003%
67	6.825	1937	1939	1941	rBV2	304	164	0.02%	0.002%
68	6.844	1941	1945	1950	rVV4	632	844	0.08%	0.009%
69	6.944	1973	1976	1978	rBV	203	125	0.01%	0.001%
70	6.989	1984	1990	1994	rBV3	349	435	0.04%	0.005%
71	7.149	2037	2040	2043	rBV2	406	222	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072118\
 Data File : VU025583.D
 Acq On : 21 Jul 2018 14:26
 Operator : MD/SY
 Sample : J4039-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

72	7.165	2043	2045	2047	rBV2	408	188	0.02%	0.002%
73	7.230	2052	2065	2088	rBV	145393	256140	24.25%	2.750%
74	7.571	2156	2171	2186	rBV	499927	867664	82.13%	9.317%
75	7.776	2233	2235	2241	rVB3	397	286	0.03%	0.003%
76	7.802	2241	2243	2247	rBV2	283	210	0.02%	0.002%
77	7.853	2247	2259	2281	rBV	97739	171253	16.21%	1.839%
78	8.185	2350	2362	2373	rBV2	14085	31537	2.99%	0.339%
79	8.313	2391	2402	2431	rVB	262693	463656	43.89%	4.979%
80	8.609	2491	2494	2498	rBV2	328	262	0.02%	0.003%
81	8.715	2524	2527	2532	rBV3	308	301	0.03%	0.003%
82	8.818	2556	2559	2560	rBV	332	156	0.01%	0.002%
83	8.924	2590	2592	2594	rBV2	263	120	0.01%	0.001%
84	8.988	2610	2612	2613	rBV2	228	76	0.01%	0.001%
85	9.091	2631	2644	2667	rBV	591458	999302	94.59%	10.730%
86	9.300	2706	2709	2713	rBV3	472	395	0.04%	0.004%
87	9.487	2763	2767	2769	rBV	294	290	0.03%	0.003%
88	9.587	2795	2798	2801	rBV	340	236	0.02%	0.003%
89	9.731	2840	2843	2845	rBV2	438	316	0.03%	0.003%
90	10.008	2927	2929	2936	rVB3	313	248	0.02%	0.003%
91	10.069	2945	2948	2953	rBV3	368	444	0.04%	0.005%
92	10.313	3022	3024	3026	rVB2	348	124	0.01%	0.001%
93	10.329	3026	3029	3030	rBV2	258	147	0.01%	0.002%
94	10.435	3049	3062	3079	rBV	325723	522153	49.42%	5.607%
95	10.615	3107	3118	3129	rBV3	5890	10053	0.95%	0.108%
96	11.085	3262	3264	3271	rVB2	552	434	0.04%	0.005%
97	11.487	3376	3389	3406	rBV	638357	1011315	95.73%	10.859%
98	11.786	3479	3482	3486	rBV4	441	292	0.03%	0.003%
99	11.863	3493	3506	3523	rBV	527584	854206	80.86%	9.172%
100	12.178	3601	3604	3607	rBV2	365	227	0.02%	0.002%


Sum of corrected areas: 9312946

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072118\
Data File : VU025583.D
Acq On : 21 Jul 2018 14:26
Operator : MD/SY
Sample : J4039-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1P6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

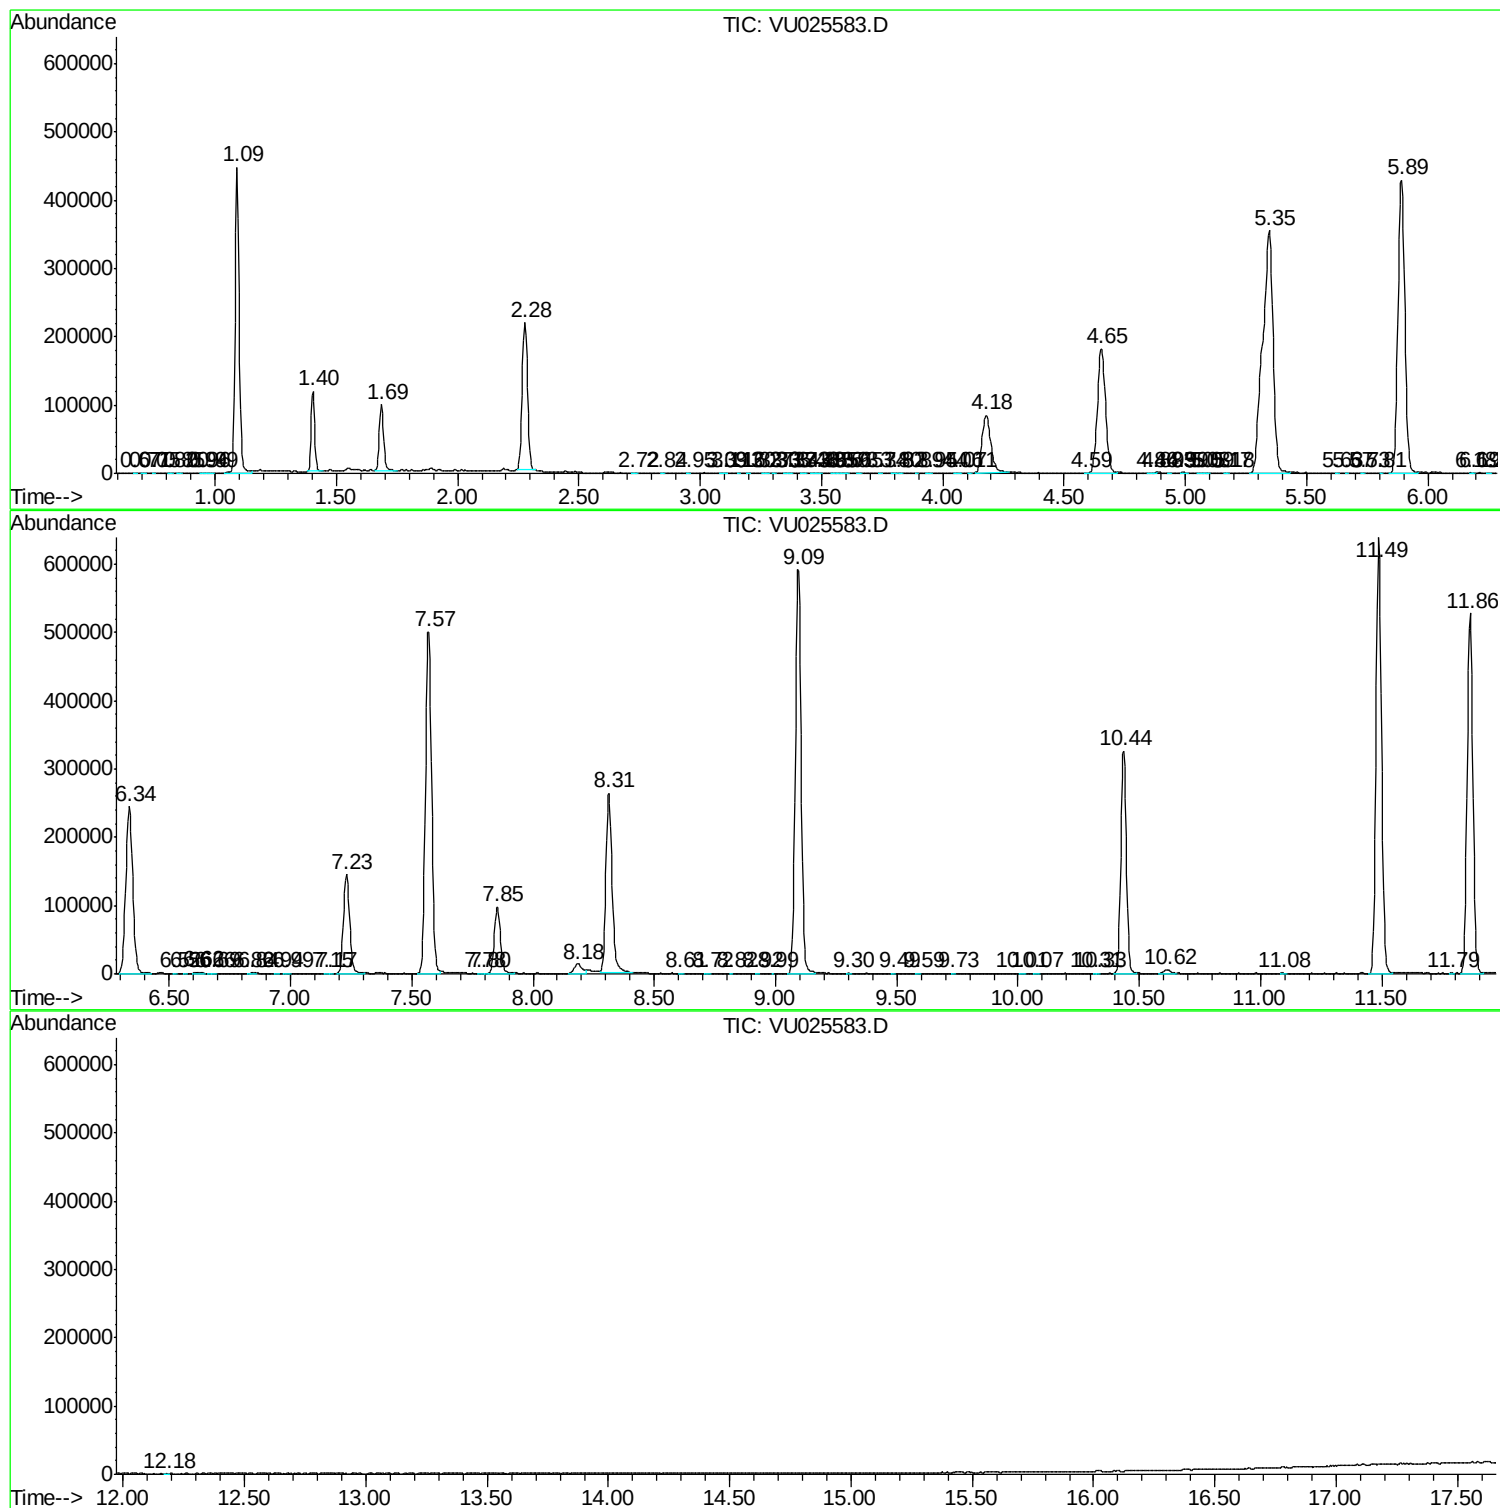

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072118\
Data File : VU025583.D
Acq On : 21 Jul 2018 14:26
Operator : MD/SY
Sample : J4039-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1P6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072118\
Data File : VU025583.D
Acq On : 21 Jul 2018 14:26
Operator : MD/SY
Sample : J4039-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1P6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc