

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072118\
 Data File : VU025585.D
 Acq On : 21 Jul 2018 15:14
 Operator : MD/SY
 Sample : J4039-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.641	12	16	19	rBV	232	151	0.01%	0.002%
2	0.661	19	22	24	rVB2	263	126	0.01%	0.001%
3	0.757	47	52	55	rBV2	195	208	0.02%	0.002%
4	0.831	68	75	78	rBV2	144	154	0.01%	0.002%
5	0.899	92	96	102	rVB2	206	213	0.02%	0.002%
6	0.937	102	108	111	rBV3	220	210	0.02%	0.002%
7	0.966	114	117	121	rBV	200	145	0.01%	0.002%
8	0.992	122	125	127	rVB2	235	124	0.01%	0.001%
9	1.011	127	131	133	rBV	238	146	0.01%	0.002%
10	1.024	133	135	137	rVB2	286	127	0.01%	0.001%
11	1.092	137	156	177	rBV	274630	327313	30.08%	3.629%
12	1.404	246	253	263	rVB	119778	122722	11.28%	1.361%
13	1.683	333	340	353	rVB	98248	122961	11.30%	1.363%
14	2.275	515	524	537	rBV	221898	333465	30.64%	3.698%
15	2.619	627	631	634	rBV3	758	618	0.06%	0.007%
16	2.796	682	686	688	rBV	496	387	0.04%	0.004%
17	2.905	718	720	724	rBV	221	133	0.01%	0.001%
18	2.947	731	733	738	rBV2	300	176	0.02%	0.002%
19	3.101	778	781	785	rBV2	390	310	0.03%	0.003%
20	3.156	792	798	801	rBV3	323	314	0.03%	0.003%
21	3.259	826	830	833	rBV3	422	347	0.03%	0.004%
22	3.281	833	837	840	rVV2	340	290	0.03%	0.003%
23	3.313	845	847	850	rVB	287	114	0.01%	0.001%
24	3.349	853	858	862	rBV3	330	279	0.03%	0.003%
25	3.387	867	870	874	rBV3	418	416	0.04%	0.005%
26	3.439	884	886	891	rVB3	240	153	0.01%	0.002%
27	3.461	891	893	897	rVB2	291	178	0.02%	0.002%
28	3.487	897	901	903	rBV2	298	238	0.02%	0.003%
29	3.506	903	907	908	rBV	158	128	0.01%	0.001%
30	3.577	923	929	934	rBV2	565	519	0.05%	0.006%
31	3.635	945	947	950	rBV	328	218	0.02%	0.002%
32	3.657	952	954	958	rVV2	349	196	0.02%	0.002%
33	3.677	958	960	964	rVB2	355	219	0.02%	0.002%
34	3.719	964	973	974	rBV2	310	334	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072118\
 Data File : VU025585.D
 Acq On : 21 Jul 2018 15:14
 Operator : MD/SY
 Sample : J4039-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	3.834	1005	1009	1011	rBV	216	151	0.01%	0.002%
36	3.998	1056	1060	1066	rVB3	460	490	0.05%	0.005%
37	4.030	1067	1070	1072	rBV2	362	239	0.02%	0.003%
38	4.111	1093	1095	1098	rBV	253	146	0.01%	0.002%
39	4.175	1100	1115	1153	rVV	89447	242770	22.31%	2.692%
40	4.532	1224	1226	1231	rVB2	457	261	0.02%	0.003%
41	4.567	1231	1237	1239	rBV4	433	411	0.04%	0.005%
42	4.654	1247	1264	1287	rBV2	188263	439677	40.40%	4.875%
43	4.783	1302	1304	1308	rVB2	500	336	0.03%	0.004%
44	4.809	1308	1312	1314	rVB	896	510	0.05%	0.006%
45	4.837	1318	1321	1322	rBV	206	104	0.01%	0.001%
46	4.876	1329	1333	1334	rBV2	594	374	0.03%	0.004%
47	4.956	1355	1358	1361	rBV3	285	232	0.02%	0.003%
48	5.034	1379	1382	1385	rVB	286	181	0.02%	0.002%
49	5.066	1385	1392	1395	rBV	211	242	0.02%	0.003%
50	5.143	1413	1416	1418	rBV	155	94	0.01%	0.001%
51	5.175	1423	1426	1429	rVB2	203	127	0.01%	0.001%
52	5.252	1447	1450	1454	rBV	171	157	0.01%	0.002%
53	5.345	1454	1479	1506	rBV2	363297	1088312	100.00%	12.068%
54	5.548	1540	1542	1545	rVB	323	130	0.01%	0.001%
55	5.571	1545	1549	1553	rBV	340	246	0.02%	0.003%
56	5.609	1558	1561	1564	rBV	217	188	0.02%	0.002%
57	5.731	1593	1599	1600	rBV	347	249	0.02%	0.003%
58	5.760	1605	1608	1611	rVB2	369	225	0.02%	0.002%
59	5.831	1627	1630	1634	rBV2	335	194	0.02%	0.002%
60	5.889	1634	1648	1672	rBV	388515	761443	69.97%	8.443%
61	6.104	1713	1715	1718	rBV2	313	214	0.02%	0.002%
62	6.133	1721	1724	1726	rBV	209	129	0.01%	0.001%
63	6.175	1734	1737	1738	rBV	473	244	0.02%	0.003%
64	6.336	1772	1787	1808	rBV	246979	493136	45.31%	5.468%
65	6.571	1857	1860	1862	rBV2	244	131	0.01%	0.001%
66	6.828	1937	1940	1941	rBV3	315	180	0.02%	0.002%
67	7.021	1997	2000	2003	rBV2	217	176	0.02%	0.002%
68	7.104	2023	2026	2029	rBV2	379	270	0.02%	0.003%
69	7.230	2053	2065	2082	rBV2	145825	258375	23.74%	2.865%
70	7.358	2100	2105	2107	rBV3	887	837	0.08%	0.009%
71	7.458	2134	2136	2139	rVB	292	159	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072118\
 Data File : VU025585.D
 Acq On : 21 Jul 2018 15:14
 Operator : MD/SY
 Sample : J4039-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

72	7.570	2157	2171	2193	rBV	512524	885670	81.38%	9.821%
73	7.760	2227	2230	2232	rVB2	640	267	0.02%	0.003%
74	7.853	2247	2259	2280	rBV	102328	176083	16.18%	1.953%
75	8.021	2309	2311	2314	rBV2	390	232	0.02%	0.003%
76	8.120	2339	2342	2344	rBV3	319	180	0.02%	0.002%
77	8.185	2352	2362	2370	rBV2	11003	22306	2.05%	0.247%
78	8.313	2391	2402	2433	rVB	277046	489853	45.01%	5.432%
79	8.525	2464	2468	2471	rBV2	750	522	0.05%	0.006%
80	8.541	2471	2473	2474	rBV	255	97	0.01%	0.001%
81	8.950	2597	2600	2603	rBV	330	227	0.02%	0.003%
82	9.017	2619	2621	2623	rBV2	240	91	0.01%	0.001%
83	9.091	2631	2644	2665	rBV	552780	909470	83.57%	10.085%
84	9.278	2700	2702	2705	rBV	365	157	0.01%	0.002%
85	9.429	2746	2749	2750	rBV	249	117	0.01%	0.001%
86	9.519	2775	2777	2779	rBV	258	135	0.01%	0.001%
87	9.644	2814	2816	2818	rBV	229	132	0.01%	0.001%
88	9.673	2822	2825	2827	rBV	234	191	0.02%	0.002%
89	9.979	2918	2920	2925	rBV2	345	322	0.03%	0.004%
90	10.030	2932	2936	2940	rVB	433	312	0.03%	0.003%
91	10.056	2940	2944	2946	rBV2	390	320	0.03%	0.004%
92	10.374	3041	3043	3045	rBV	302	155	0.01%	0.002%
93	10.435	3050	3062	3077	rVV	341146	540444	49.66%	5.993%
94	10.702	3143	3145	3146	rBV	403	184	0.02%	0.002%
95	10.850	3186	3191	3195	rBV3	355	416	0.04%	0.005%
96	11.156	3283	3286	3287	rBV2	331	216	0.02%	0.002%
97	11.184	3292	3295	3297	rBV	441	290	0.03%	0.003%
98	11.487	3377	3389	3406	rBV	579168	918629	84.41%	10.186%
99	11.728	3460	3464	3466	rBV2	374	313	0.03%	0.003%
100	11.863	3493	3506	3526	rBV	539659	865943	79.57%	9.602%


Sum of corrected areas: 9018246

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072118\
Data File : VU025585.D
Acq On : 21 Jul 2018 15:14
Operator : MD/SY
Sample : J4039-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1P7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

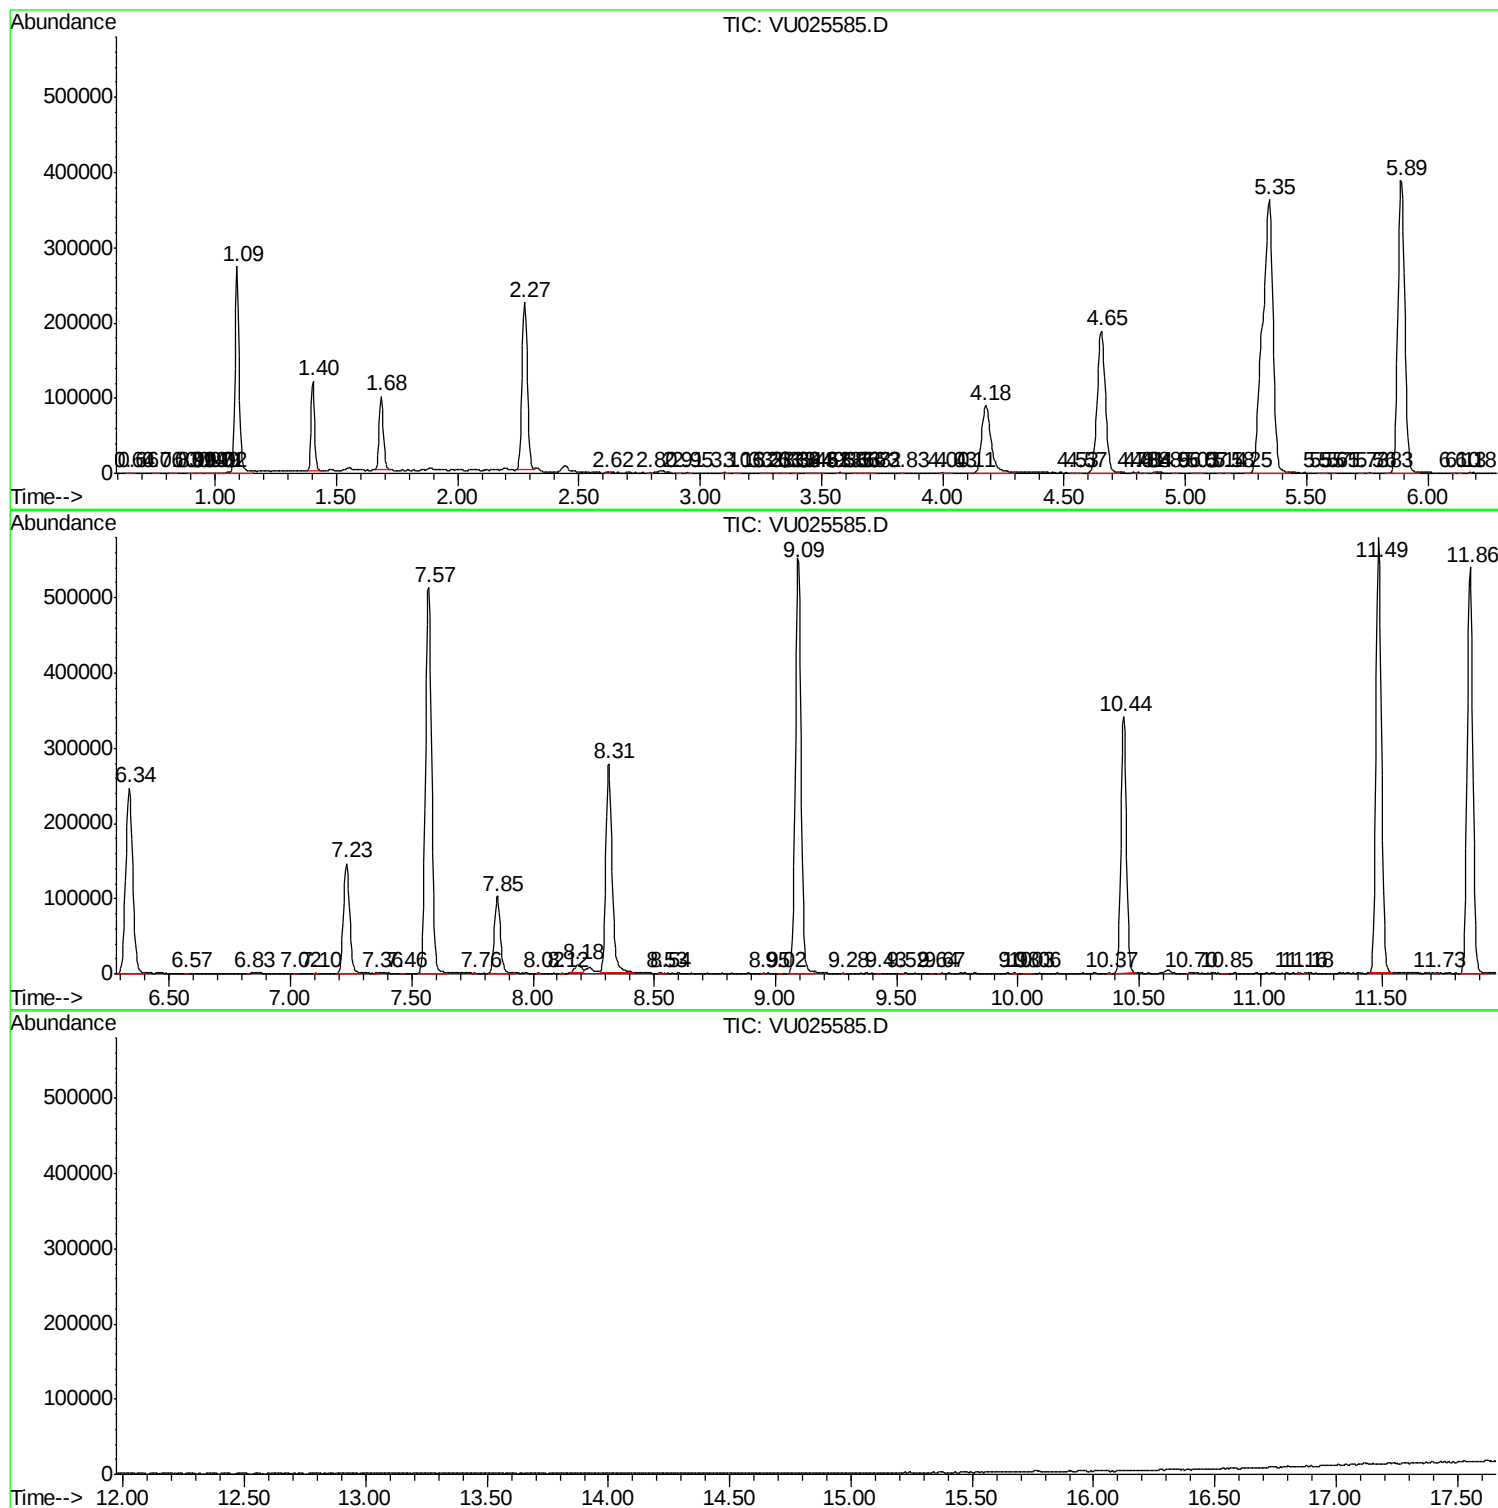

Data_Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072118\
Data_File : VU025585.D
Acq_On : 21-Jul-2018 15:144
Operator : MD/SYY
Sample : J4039-099
Misc : 5.0mL/MSVOA_U/WATER
ALS_Vial : 15 Sample_Multiplier: 11

Instrument :
MSVOA_U
ClientSampleId :
DB1P7

Quant_Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
