

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072118\
 Data File : VU025589.D
 Acq On : 21 Jul 2018 17:10
 Operator : MD/SY
 Sample : J4065-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.635	8	14	16	rBV2	238	246	0.002%	0.0002%
2	0.719	36	40	41	rBV2	191	145	0.001%	0.0001%
3	0.805	64	67	69	rBV2	176	104	0.001%	0.0001%
4	0.841	74	78	84	rBV2	206	195	0.002%	0.0002%
5	0.876	84	89	91	rBV	245	201	0.002%	0.0002%
6	0.902	95	97	99	rBV	271	131	0.001%	0.0001%
7	0.953	109	113	114	rBV	296	202	0.002%	0.0002%
8	1.027	133	136	137	rBV	120	71	0.001%	0.0001%
9	1.088	147	155	175	rBV	1140452	1270437	100.00%	12.744%
10	1.404	246	253	263	rBV	116356	121816	9.59%	1.222%
11	1.683	333	340	357	rVB	97851	126070	9.92%	1.265%
12	2.275	515	524	537	rVB	221655	338142	26.62%	3.392%
13	2.558	608	612	615	rBV2	720	595	0.005%	0.0006%
14	2.976	740	742	744	rBV3	480	299	0.002%	0.0003%
15	3.548	915	920	923	rBV3	370	393	0.003%	0.0004%
16	3.567	923	926	930	rVV	523	363	0.003%	0.0004%
17	3.587	930	932	936	rVB3	232	165	0.001%	0.0002%
18	3.664	954	956	961	rBV	604	397	0.003%	0.0004%
19	3.873	1018	1021	1023	rBV	238	168	0.001%	0.0002%
20	3.931	1036	1039	1042	rBV2	197	157	0.001%	0.0002%
21	3.976	1050	1053	1055	rBV2	145	69	0.001%	0.0001%
22	4.178	1101	1116	1148	rBV	94237	243095	19.13%	2.439%
23	4.548	1228	1231	1233	rBV2	216	108	0.001%	0.0001%
24	4.654	1245	1264	1287	rBV	190422	442723	34.85%	4.441%
25	4.767	1296	1299	1301	rBV2	402	274	0.002%	0.0003%
26	4.953	1352	1357	1363	rVB2	295	312	0.002%	0.0003%
27	5.037	1380	1383	1384	rBV	209	110	0.001%	0.0001%
28	5.230	1441	1443	1446	rBV	187	99	0.001%	0.0001%
29	5.346	1454	1479	1507	rBV2	363892	1087070	85.57%	10.905%
30	5.535	1535	1538	1540	rBV2	347	234	0.002%	0.0002%
31	5.606	1558	1560	1561	rVB	218	67	0.001%	0.0001%
32	5.616	1561	1563	1566	rBV	185	96	0.001%	0.0001%
33	5.670	1575	1580	1582	rBV2	473	454	0.004%	0.0005%
34	5.728	1595	1598	1599	rBV2	298	155	0.001%	0.0002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072118\
 Data File : VU025589.D
 Acq On : 21 Jul 2018 17:10
 Operator : MD/SY
 Sample : J4065-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	5.892	1631	1649	1675	rBV	379742	745012	58.64%	7.474%
36	6.127	1719	1722	1724	rVB	292	150	0.01%	0.002%
37	6.143	1724	1727	1728	rBV2	202	115	0.01%	0.001%
38	6.175	1731	1737	1739	rBV3	1096	993	0.08%	0.010%
39	6.210	1746	1748	1750	rBV2	173	92	0.01%	0.001%
40	6.336	1772	1787	1811	rBV	248786	498931	39.27%	5.005%
41	6.603	1868	1870	1872	rBV	243	133	0.01%	0.001%
42	6.728	1905	1909	1915	rBV2	376	383	0.03%	0.004%
43	6.760	1915	1919	1921	rBV2	313	190	0.01%	0.002%
44	6.834	1940	1942	1944	rBV	270	119	0.01%	0.001%
45	7.001	1991	1994	1997	rBV	438	292	0.02%	0.003%
46	7.230	2053	2065	2085	rBV	146002	262880	20.69%	2.637%
47	7.464	2135	2138	2139	rBV2	385	225	0.02%	0.002%
48	7.567	2157	2170	2189	rBV	513517	883282	69.53%	8.861%
49	7.853	2246	2259	2278	rBV	104547	181211	14.26%	1.818%
50	8.014	2306	2309	2312	rBV3	445	236	0.02%	0.002%
51	8.188	2350	2363	2372	rBV3	8997	21280	1.68%	0.213%
52	8.313	2391	2402	2438	rVB	294856	513837	40.45%	5.155%
53	8.696	2517	2521	2522	rBV	337	249	0.02%	0.002%
54	8.725	2527	2530	2534	rVV2	478	374	0.03%	0.004%
55	8.789	2548	2550	2553	rBV	303	192	0.02%	0.002%
56	9.091	2631	2644	2665	rBV	538759	884416	69.62%	8.872%
57	9.249	2690	2693	2703	rVB5	608	837	0.07%	0.008%
58	9.374	2728	2732	2733	rBV	575	339	0.03%	0.003%
59	9.738	2843	2845	2847	rBV	256	138	0.01%	0.001%
60	10.435	3049	3062	3080	rBV	343085	547561	43.10%	5.493%
61	10.619	3109	3119	3130	rVB4	2833	4983	0.39%	0.050%
62	11.487	3376	3389	3410	rBV	570904	900206	70.86%	9.030%
63	11.863	3493	3506	3524	rBV	555487	884296	69.61%	8.871%
64	12.892	3821	3826	3827	rBV2	584	509	0.04%	0.005%




Sum of corrected areas: 9968624

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072118\
Data File : VU025589.D
Acq On : 21 Jul 2018 17:10
Operator : MD/SY
Sample : J4065-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

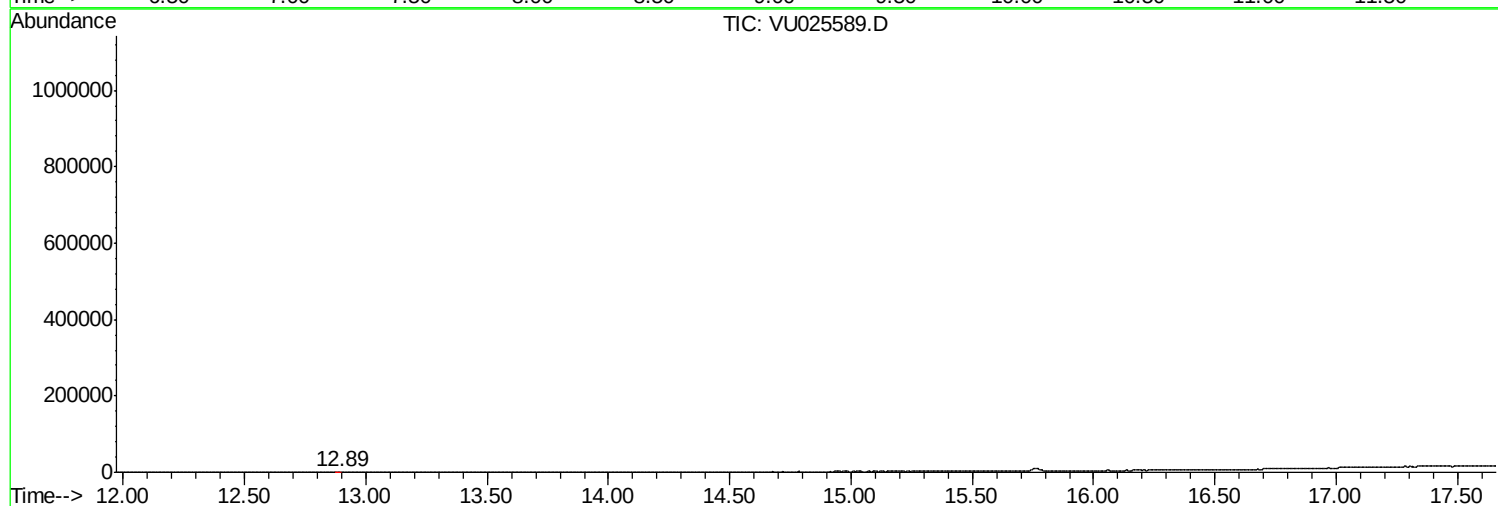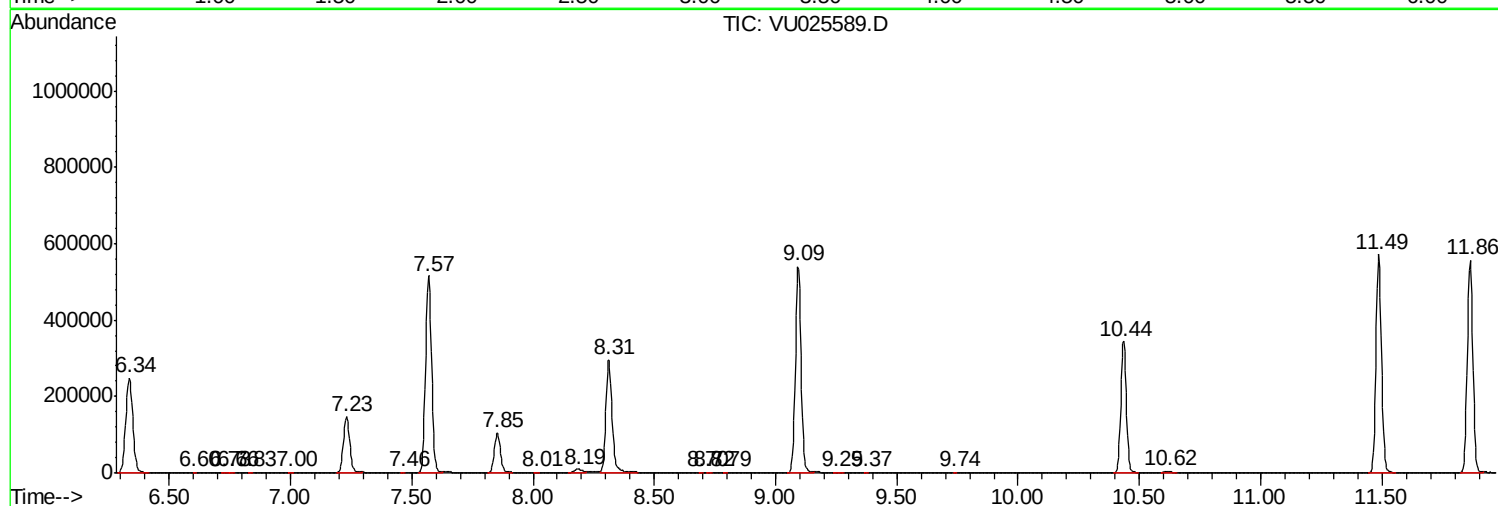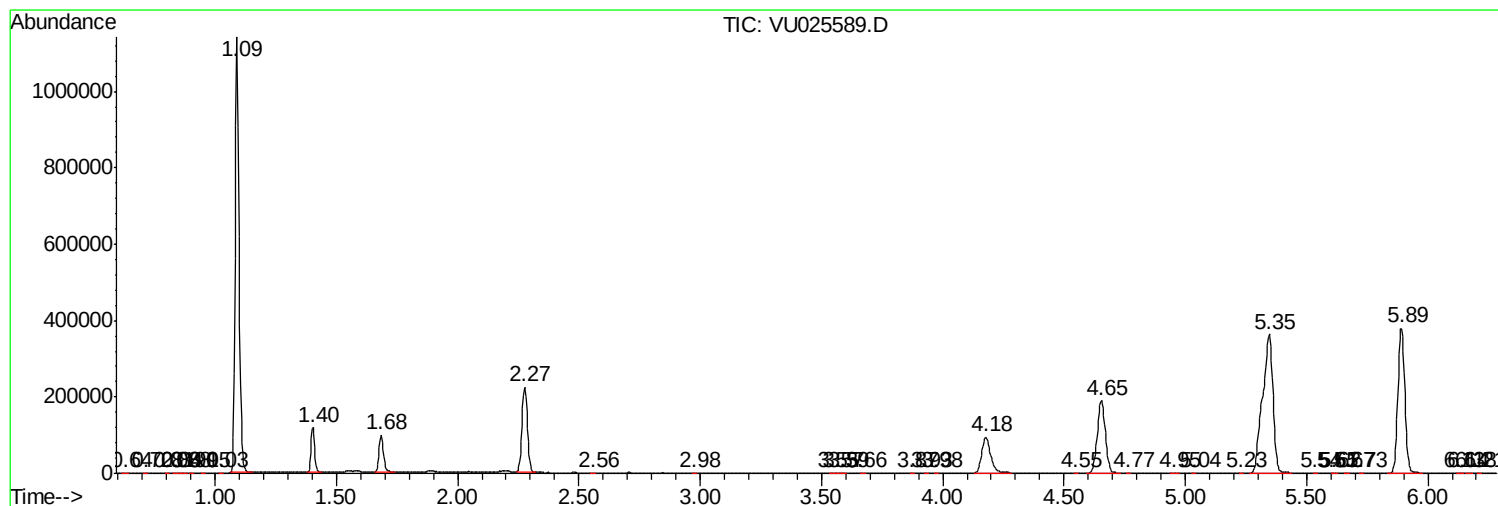

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072118\
Data_File : VU025589.D
Acq_On : 21-Jul-2018 17:100
Operator : MD/SYY
Sample : J4065-144
Misc : 5.0mL/MSVOA_U/WATER
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
