


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072118\
Data File : VU025571.D
Acq On : 21 Jul 2018 09:21
Operator : MD/SY
Sample : BFB47
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Title : VOC Analysis
Last Update : Tue Jul 24 02:07:37 2018

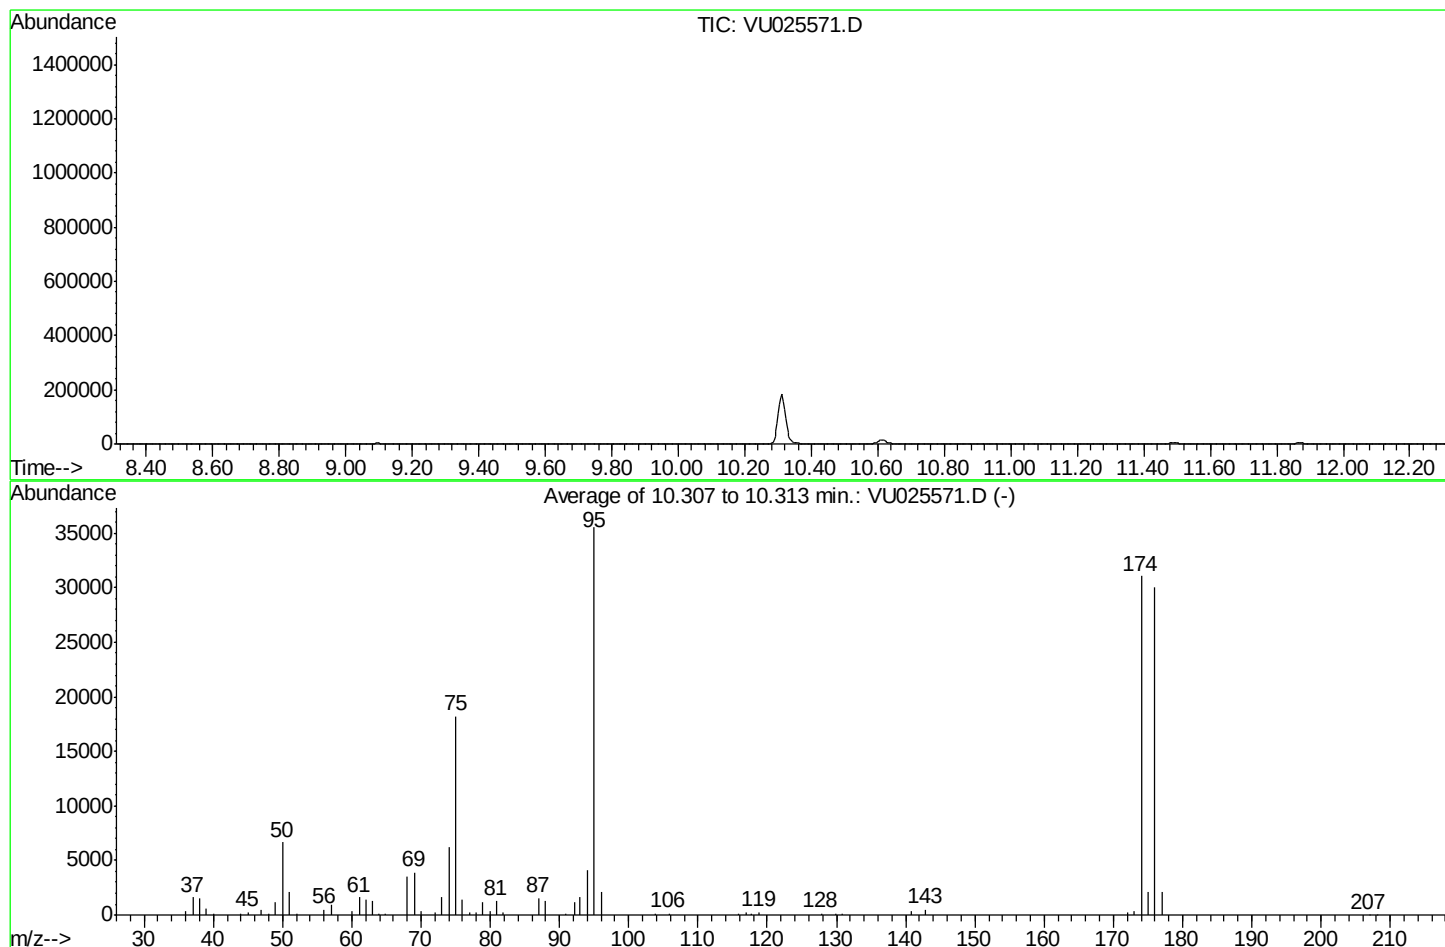

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	6655	PASS
75	95	30	80	51.2	18192	PASS
95	95	100	100	100.0	35530	PASS
96	95	5	9	5.9	2083	PASS
173	174	0.00	2	1.1	350	PASS
174	95	50	120	87.4	31053	PASS
175	174	5	9	6.9	2140	PASS
176	174	95	101	96.7	30013	PASS
177	176	5	9	7.0	2089	PASS

Scan 3011 (10.271 min): VU025571.D
BFB47

m/z	Abundance
43.90	418.0
207.10	323.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	317.0
37.00	1536.0
38.00	1505.0
39.00	619.0
40.00	100.0
44.00	567.0
45.00	311.0
46.90	492.0
47.90	147.0
49.00	1131.0
50.00	6777.0
51.00	2015.0
52.00	102.0
56.00	531.0
57.00	937.0
60.00	285.0
61.10	1549.0
62.00	1463.0
63.00	1244.0
63.90	162.0
64.80	140.0
68.00	3481.0
69.00	3973.0
70.00	276.0
72.00	195.0
73.00	1612.0
74.00	5912.0
75.00	17904.0
76.00	1318.0
77.00	222.0
78.00	252.0
78.90	1225.0
80.00	373.0
80.90	1325.0
81.90	307.0
87.00	1532.0
87.90	1281.0
90.90	174.0
92.10	1243.0
93.00	1629.0
94.00	4315.0
95.00	34008.0
96.00	2135.0
103.80	149.0
105.80	180.0
115.80	125.0
116.90	191.0
117.70	167.0
119.00	213.0
127.80	153.0
129.90	145.0
140.80	383.0
142.90	492.0
172.00	277.0
173.00	321.0
174.00	29656.0
174.90	2103.0
176.00	28056.0
177.00	2065.0
206.90	393.0
208.10	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	337.0
37.00	1660.0
38.00	1592.0
39.00	644.0
40.10	134.0
44.00	514.0
45.00	291.0
47.00	535.0
48.00	172.0
49.00	1263.0
50.00	6939.0
51.00	2219.0
52.00	139.0
56.00	517.0
57.00	965.0
60.00	366.0
61.00	1660.0
62.00	1472.0
63.00	1269.0
63.90	188.0
64.80	154.0
68.00	3616.0
69.00	4036.0
70.00	348.0
72.00	197.0
73.00	1739.0
74.00	6328.0
75.00	18696.0
76.00	1471.0
77.00	264.0
77.90	213.0
78.90	1269.0
79.90	363.0
80.90	1359.0
81.90	282.0
87.00	1611.0
87.90	1306.0
90.90	137.0
92.10	1255.0
93.00	1701.0
94.00	4296.0
95.00	36800.0
96.00	2088.0
103.80	175.0
105.80	170.0
115.90	135.0
116.90	186.0
117.70	166.0
119.00	267.0
127.90	168.0
129.90	150.0
130.90	111.0
140.80	398.0
142.90	501.0
172.00	312.0
173.00	358.0
174.00	31936.0
174.90	2162.0
176.00	30912.0
177.00	2150.0
206.90	393.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	292.0
37.00	1665.0
38.00	1615.0
39.00	652.0
40.00	166.0
44.00	491.0
44.90	274.0
47.00	452.0
48.00	179.0
49.00	1279.0
50.00	6250.0
51.00	2275.0
52.00	128.0
56.00	505.0
57.00	970.0
60.00	398.0
61.00	1690.0
62.00	1422.0
63.00	1205.0
63.90	143.0
64.80	143.0
68.00	3442.0
69.00	3744.0
69.90	337.0
72.00	177.0
73.00	1670.0
74.00	6315.0
75.00	17976.0
76.00	1435.0
77.00	235.0
77.90	163.0
78.90	1143.0
79.90	316.0
80.90	1348.0
81.90	257.0
87.00	1560.0
87.90	1311.0
90.90	104.0
92.10	1057.0
93.00	1561.0
94.00	3895.0
95.00	35784.0
96.00	2028.0
103.90	184.0
105.90	171.0
116.00	129.0
116.90	174.0
117.80	123.0
118.80	314.0
127.90	165.0
129.80	156.0
130.90	102.0
140.80	320.0
142.90	474.0
172.00	288.0
173.00	373.0
174.00	31568.0
175.00	2157.0
176.00	31072.0
177.00	2053.0
207.00	370.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47