

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072121\
 Data File : VU044379.D
 Acq On : 21 Jul 2021 13:19
 Operator : SY/MD
 Sample : M3035-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-EDBCP-WS

Quant Time: Jul 22 05:02:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 16 14:36:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.121	96	49838	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.639	95	18229	0.906	ug/l	0.00
Spiked Amount 1.000			Recovery	=	91.000%	
68) 1,2-Dichlorobenzene-d4	12.201	152	18222	0.929	ug/l	0.00
Spiked Amount 1.000			Recovery	=	93.000%	
Target Compounds						
						Qvalue
15) Methylene Chloride	3.051	84	32479	1.798	ug/l	98
56) 1,2-Dibromoethane	8.932	107	8995	0.807	ug/l	96
71) 1,2,3-Trichloropropane	10.832	75	14587	1.131	ug/l	83
86) 1,2-Dibromo-3-Chloropr...	13.005	75	3841	1.477	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072121\
Data File : VU044379.D
Acq On : 21 Jul 2021 13:19
Operator : SY/MD
Sample : M3035-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Quant Time: Jul 22 05:02:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 16 14:36:39 2021
Response via : Initial Calibration

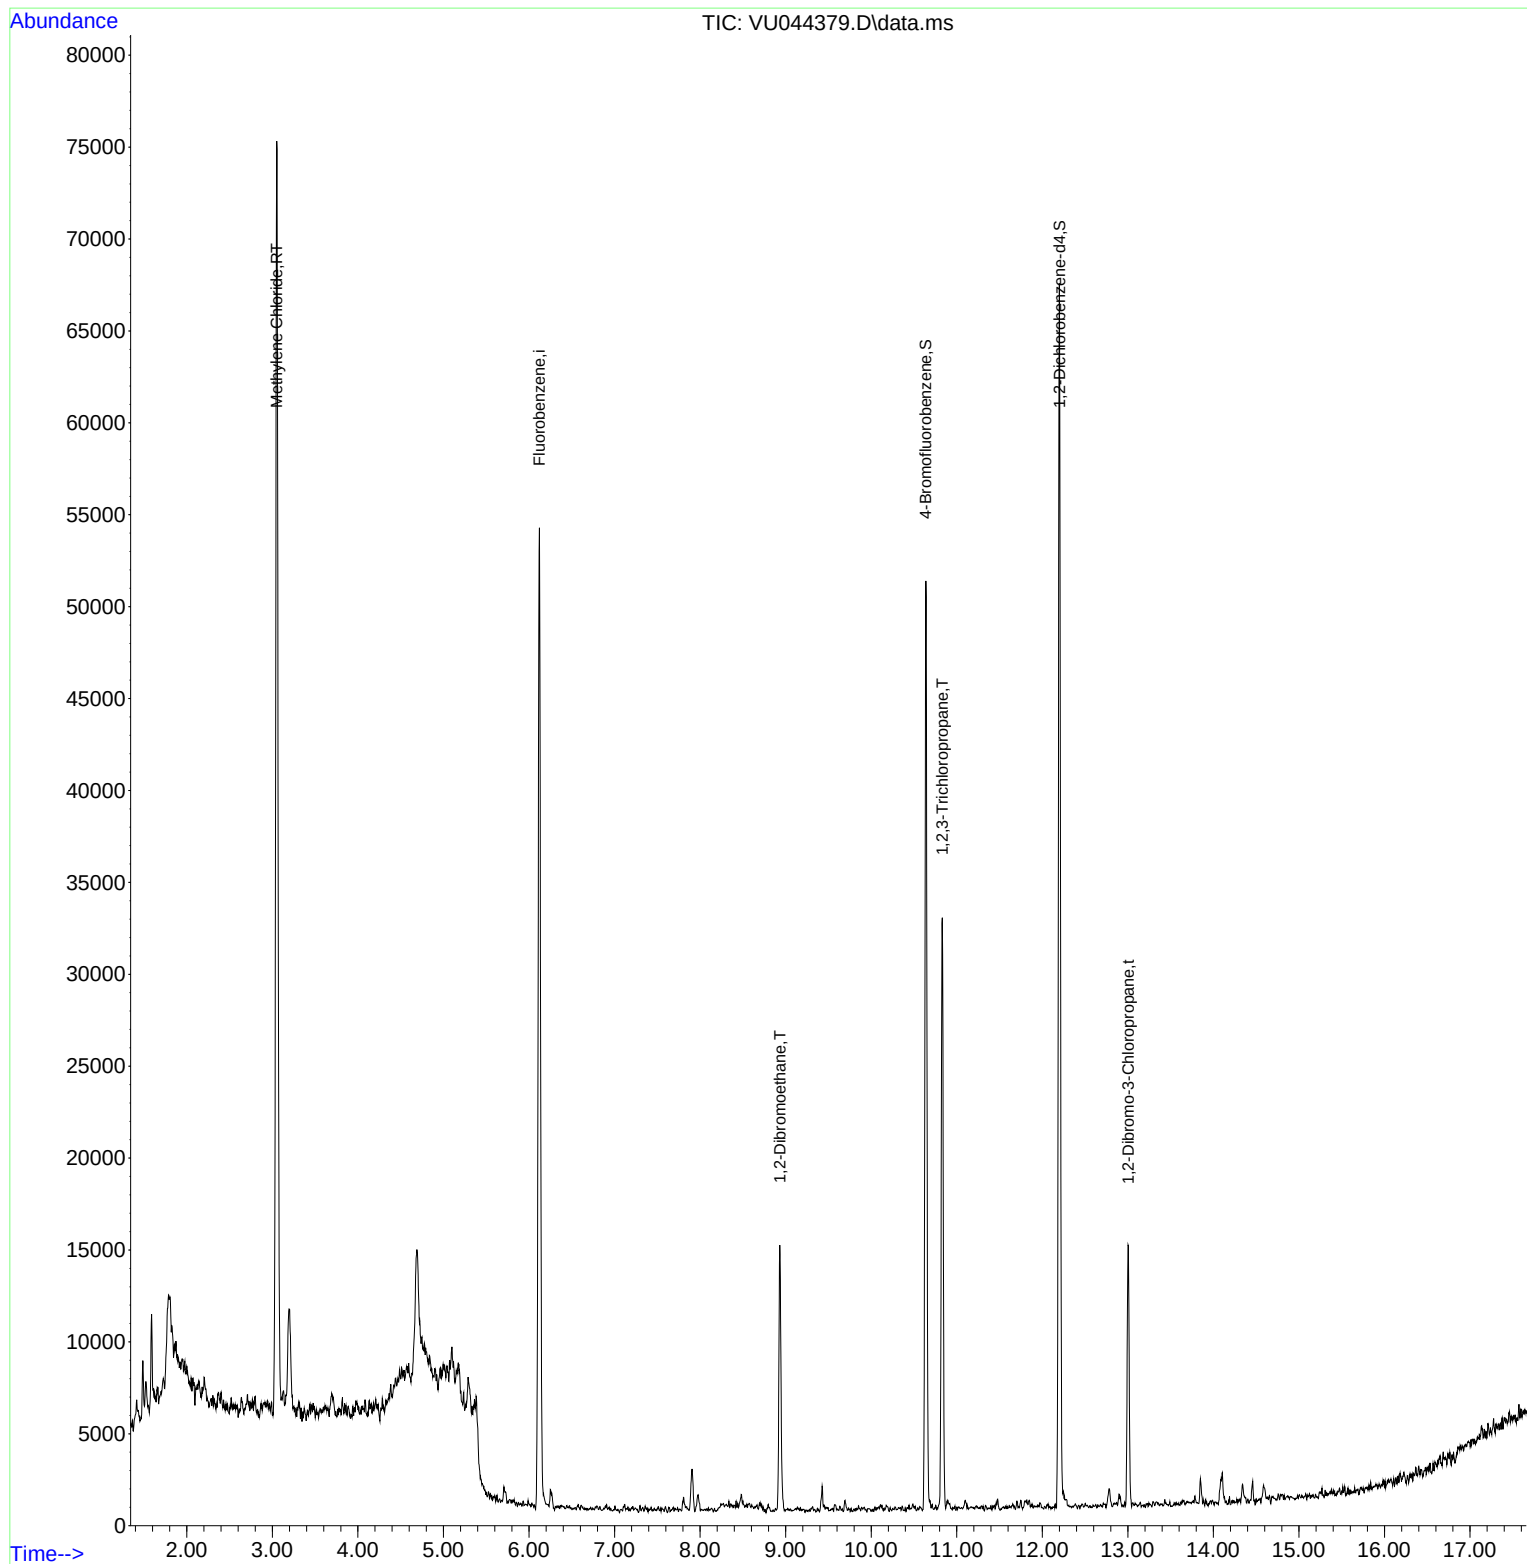




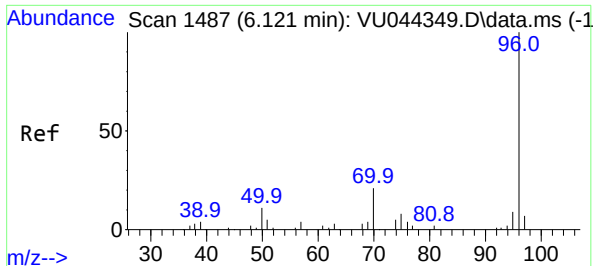


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.121 min Scan# 1487
Delta R.T. 0.000 min
Lab File: VU044379.D
Acq: 21 Jul 2021 13:19

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Tgt Ion: 96 Resp: 49838




Ion	Ratio	Lower	Upper
96	100		
70	21.0	16.2	24.2
95	8.4	7.3	10.9
97	6.3	0.0	0.0#

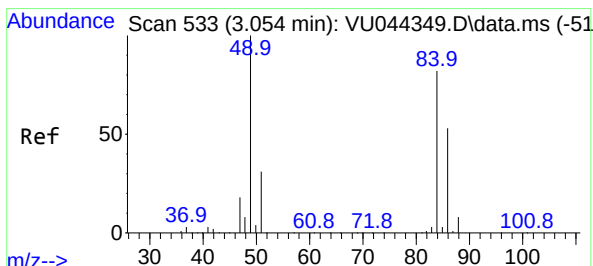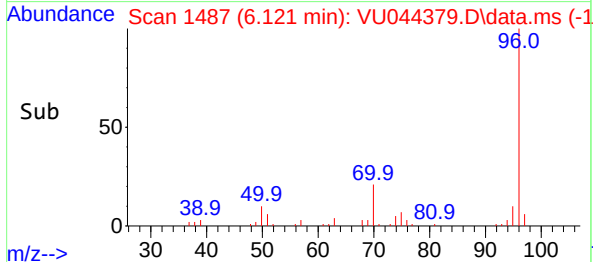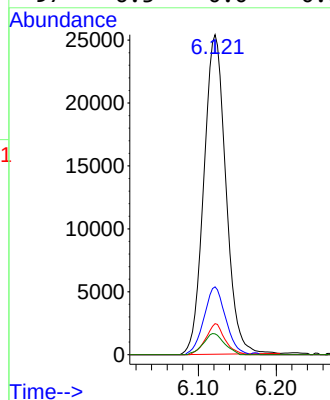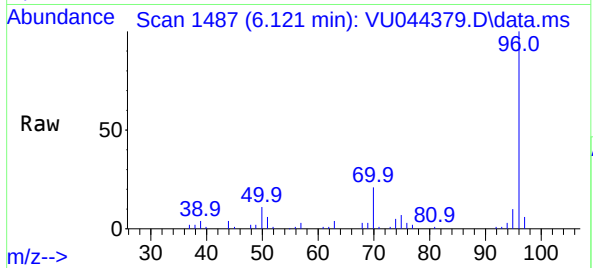


#15
Methylene Chloride
Concen: 1.798 ug/l
RT: 3.051 min Scan# 532
Delta R.T. -0.003 min
Lab File: VU044379.D
Acq: 21 Jul 2021 13:19

Tgt Ion: 84 Resp: 32479

Ion	Ratio	Lower	Upper
84	100		
49	131.2	106.3	159.5
51	39.2	0.0	81.8
86	65.5	51.4	77.0


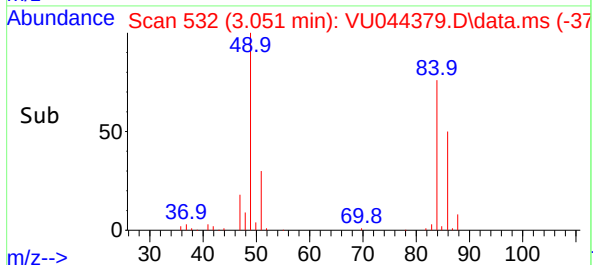
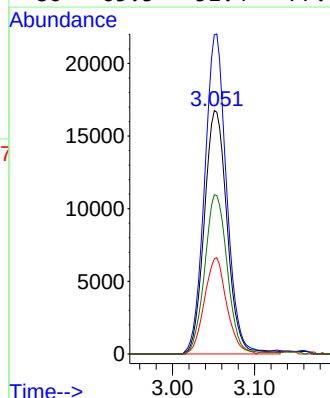
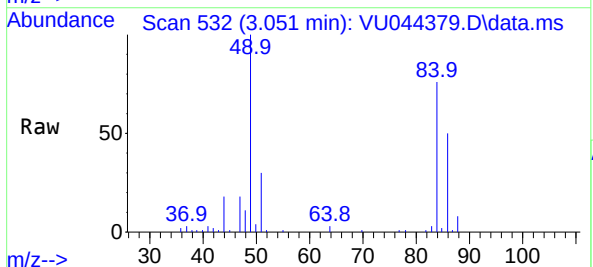


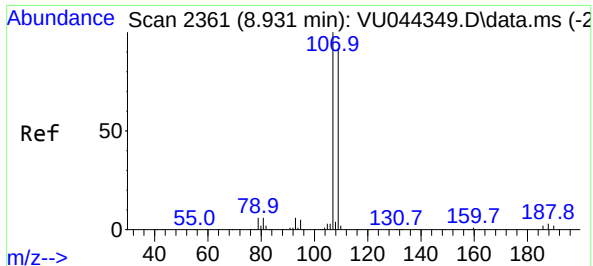

#56
1,2-Dibromoethane
Concen: 0.807 ug/l
RT: 8.932 min Scan# 2361
Delta R.T. 0.000 min
Lab File: VU044379.D
Acq: 21 Jul 2021 13:19




Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS


Tgt Ion:107 Resp: 8995
Ion Ratio Lower Upper
107 100
109 90.5 0.0 189.0

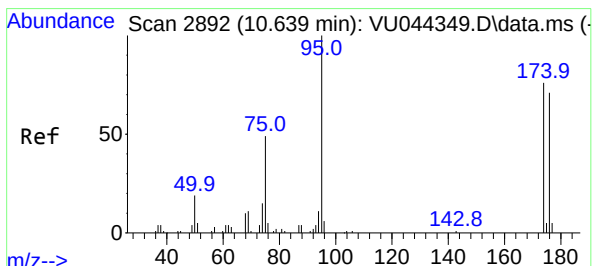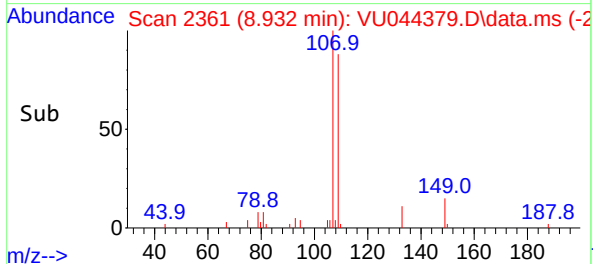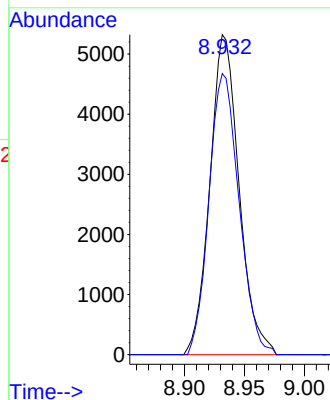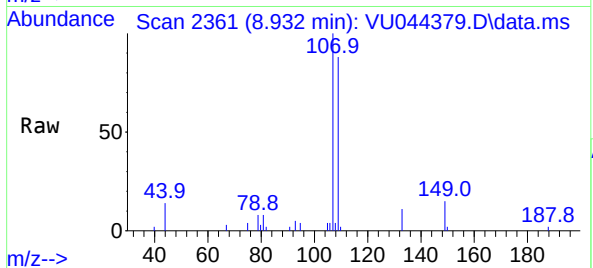

#57
4-Bromofluorobenzene
Concen: 0.906 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.000 min
Lab File: VU044379.D
Acq: 21 Jul 2021 13:19

Tgt Ion: 95 Resp: 18229
Ion Ratio Lower Upper
95 100
174 73.6 62.2 93.2
176 70.8 60.3 90.5


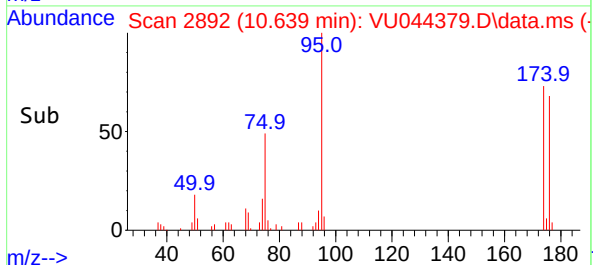
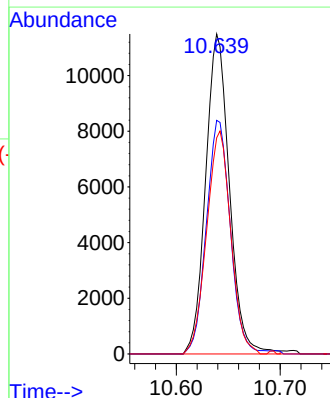
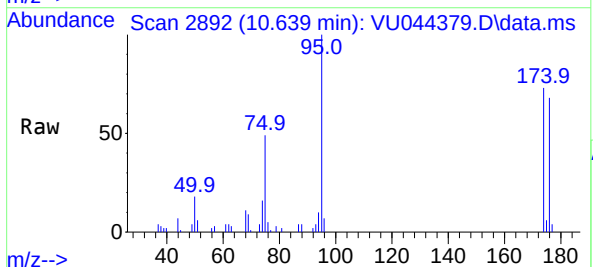


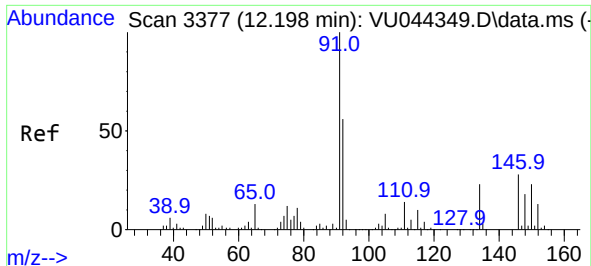

#68
1,2-Dichlorobenzene-d4
Concen: 0.929 ug/l
RT: 12.201 min Scan# 3378
Delta R.T. 0.003 min
Lab File: VU044379.D
Acq: 21 Jul 2021 13:19




Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS


Tgt Ion:152 Resp: 18222
Ion Ratio Lower Upper
152 100
115 66.9 0.0 257.0
150 158.9 0.0 630.2

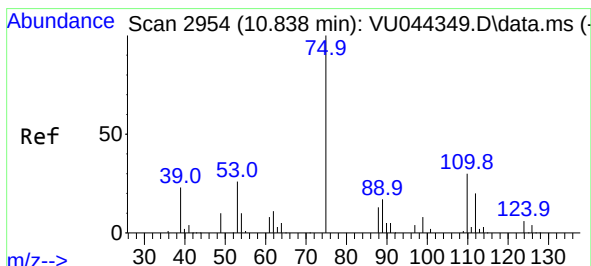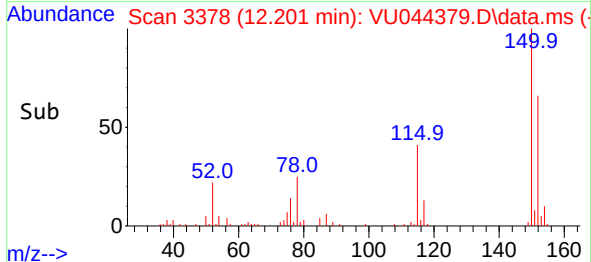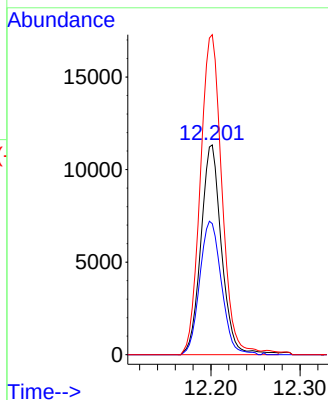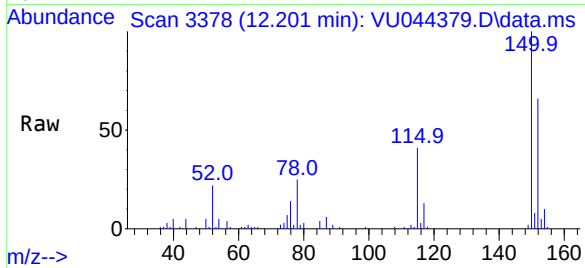

#71
1,2,3-Trichloropropane
Concen: 1.131 ug/l
RT: 10.832 min Scan# 2952
Delta R.T. -0.006 min
Lab File: VU044379.D
Acq: 21 Jul 2021 13:19


Tgt Ion: 75 Resp: 14587
Ion Ratio Lower Upper
75 100
77 31.7 0.0 111.4
110 36.8 0.0 74.6
97 17.7 0.0 35.8

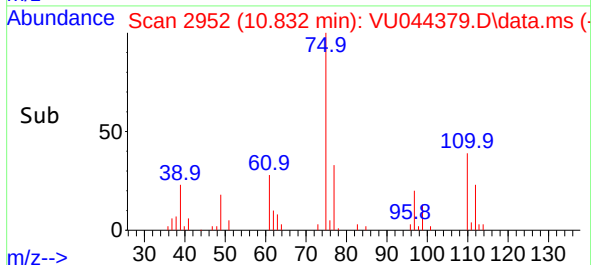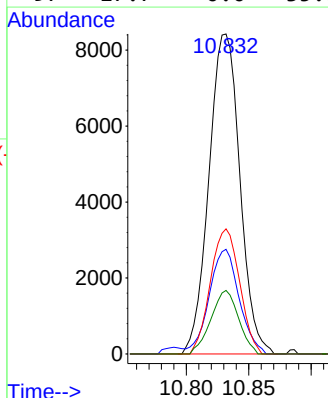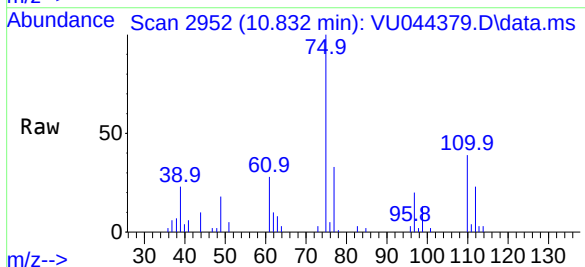

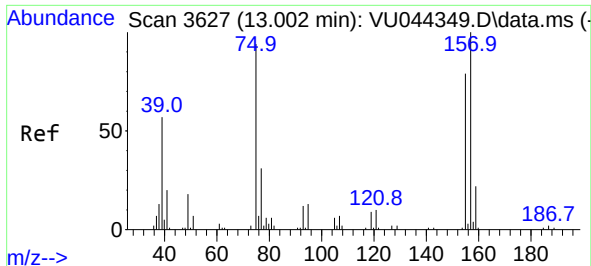

#86
 1,2-Dibromo-3-Chloropropane
 Concen: 1.477 ug/l
 RT: 13.005 min Scan# 3628
 Delta R.T. 0.003 min
 Lab File: VU044379.D
 Acq: 21 Jul 2021 13:19

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-EDBCP-WS

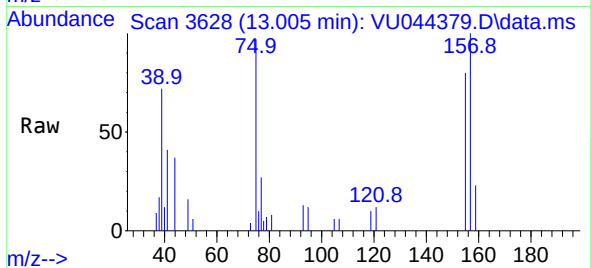

Tgt Ion: 75 Resp: 3841
 Ion Ratio Lower Upper
 75 100
 155 73.6 64.7 97.1
 157 102.7 85.3 127.9

