

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072121\
 Data File : VU044376.D
 Acq On : 21 Jul 2021 10:33
 Operator : SY/MD
 Sample : VU0721WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0721WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.044	521	530	546	rBV	13240	24678	21.20%	6.247%
2	5.710	1349	1359	1369	rVB3	1059	1879	1.61%	0.476%
3	6.118	1473	1486	1504	rBV	52557	102717	88.24%	26.000%
4	6.259	1521	1530	1537	rVB2	1085	1474	1.27%	0.373%
5	7.224	1821	1830	1832	rBV3	1163	1495	1.28%	0.378%
6	7.809	1999	2012	2020	rBV5	1562	2561	2.20%	0.648%
7	7.906	2033	2042	2050	rVB3	1632	2855	2.45%	0.723%
8	8.481	2214	2221	2232	rBV3	800	1564	1.34%	0.396%
9	8.706	2284	2291	2293	rBV3	1117	1431	1.23%	0.362%
10	9.426	2505	2515	2520	rBV3	886	1238	1.06%	0.313%
11	10.121	2721	2731	2741	rVB4	1019	1790	1.54%	0.453%
12	10.639	2881	2892	2906	rBV	51384	84427	72.53%	21.370%
13	10.793	2932	2940	2945	rBV2	873	1171	1.01%	0.296%
14	11.102	3026	3036	3044	rVB4	1054	2106	1.81%	0.533%
15	11.478	3145	3153	3163	rBV3	935	1290	1.11%	0.327%
16	11.754	3233	3239	3245	rVB2	1140	1441	1.24%	0.365%
17	11.799	3245	3253	3257	rBV2	890	1279	1.10%	0.324%
18	11.841	3260	3266	3274	rVB4	1432	2012	1.73%	0.509%
19	12.201	3367	3378	3392	rBV	69635	116405	100.00%	29.465%
20	12.896	3586	3594	3601	rBV6	3597	5565	4.78%	1.409%
21	13.847	3882	3890	3902	rVB5	4198	6639	5.70%	1.680%
22	13.992	3930	3935	3941	rBV5	1311	1594	1.37%	0.403%
23	14.028	3941	3946	3952	rVB4	1351	1317	1.13%	0.333%
24	14.095	3952	3967	3978	rBV2	6628	12346	10.61%	3.125%
25	14.339	4034	4043	4052	rBV4	4546	7494	6.44%	1.897%
26	14.455	4070	4079	4089	rBV5	2080	3220	2.77%	0.815%
27	14.584	4110	4119	4126	rBV4	1921	3080	2.65%	0.780%


Sum of corrected areas: 395068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072121\
Data File : VU044376.D
Acq On : 21 Jul 2021 10:33
Operator : SY/MD
Sample : VU0721WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0721WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

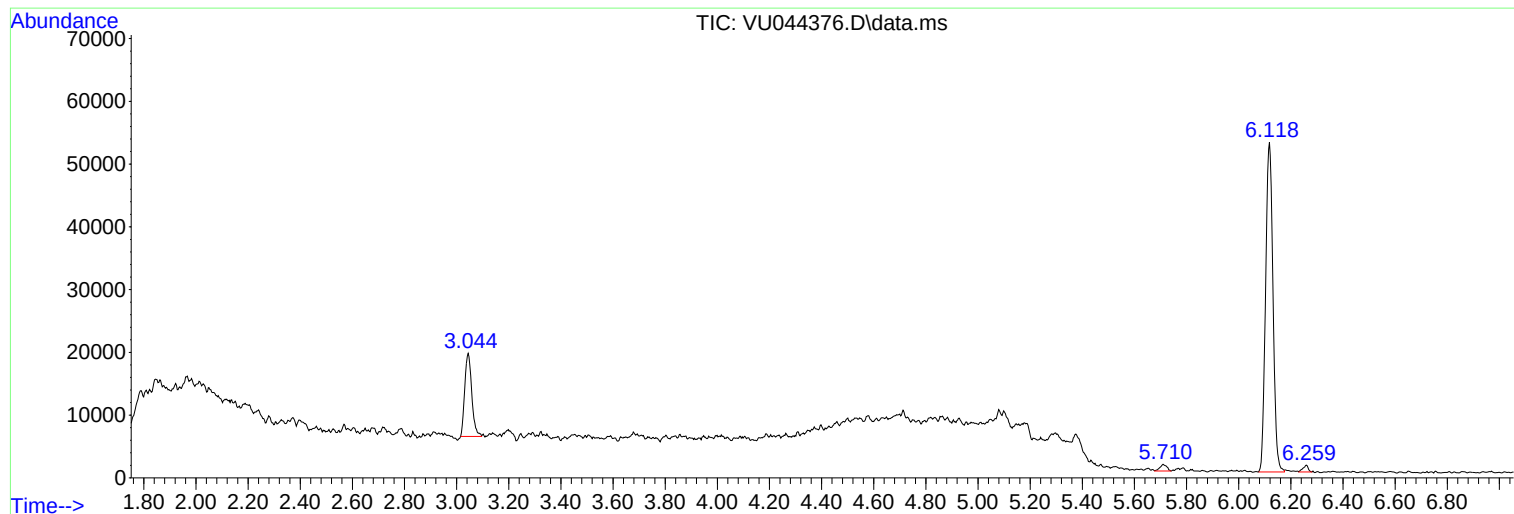

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072121\
Data File : VU044376.D
Acq On : 21 Jul 2021 10:33
Operator : SY/MD
Sample : VU0721WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0721WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072121\
Data File : VU044376.D
Acq On : 21 Jul 2021 10:33
Operator : SY/MD
Sample : VU0721WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0721WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------