
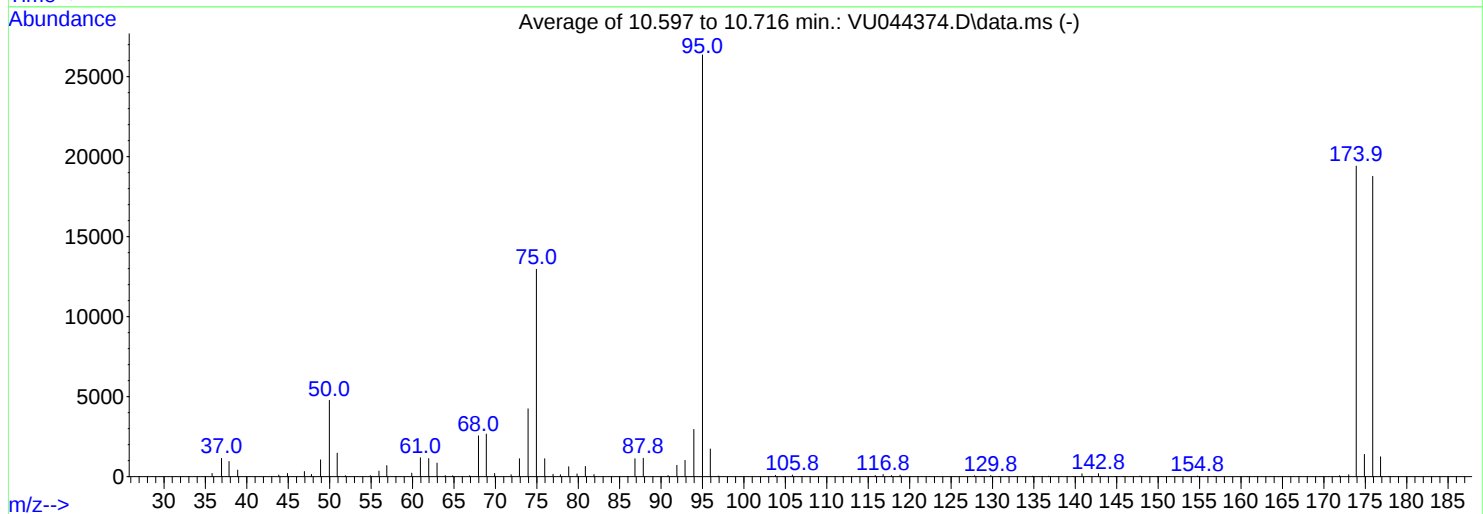


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072121\
Data File : VU044374.D
Acq On : 21 Jul 2021 08:19
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Jul 16 14:36:39 2021

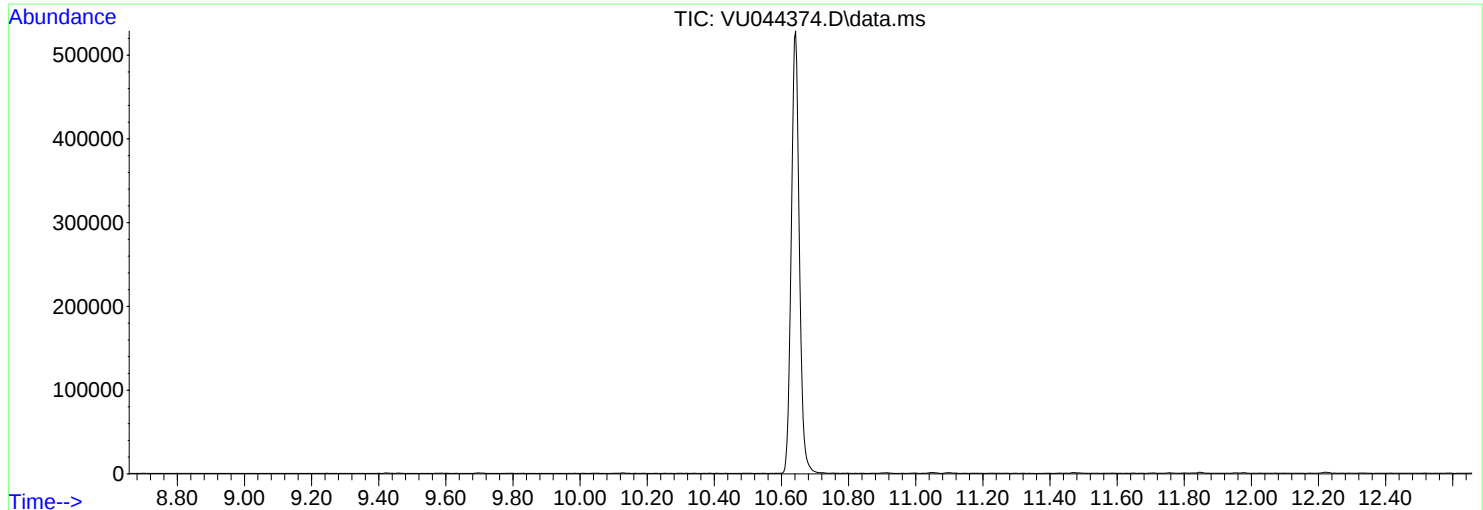

AutoFind: Averaged scan 2879 to 2916; Bkg corrected with scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	4767	PASS
75	95	30	60	49.1	12956	PASS
95	95	100	100	100.0	26362	PASS
96	95	5	9	6.6	1727	PASS
173	174	0.00	2	0.6	121	PASS
174	95	50	100	73.6	19413	PASS
175	174	5	9	7.1	1388	PASS
176	174	95	101	96.7	18767	PASS
177	176	5	9	6.6	1241	PASS