

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049824.D
 Acq On : 21 Jul 2022 13:00
 Operator : SY/MD
 Sample : N3792-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN4

Quant Time: Jul 22 04:12:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 22 03:08:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	176927	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	167408	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	70130	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	60587	40.586	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.180%
7) Chloroethane-d5	1.900	69	49572	45.940	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.880%
11) 1,1-Dichloroethene-d2	2.562	63	79088	29.993	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.980%#
21) 2-Butanone-d5	4.620	46	143095	112.287	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.290%
24) Chloroform-d	5.063	84	125702	47.542	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.080%
26) 1,2-Dichloroethane-d4	5.700	65	90875	50.783	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.560%
32) Benzene-d6	5.726	84	231573	45.533	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.060%
36) 1,2-Dichloropropane-d6	6.690	67	85869	50.197	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.400%
41) Toluene-d8	7.899	98	184261	41.604	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.200%
43) trans-1,3-Dichloroprop...	8.179	79	33318	46.228	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.460%
47) 2-Hexanone-d5	8.632	63	72507	94.227	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.230%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	122336	51.110	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.220%
66) 1,2-Dichlorobenzene-d4	12.195	152	62668	47.395	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.780%
Target Compounds						
13) Acetone	2.626	43	3509	2.897	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049824.D
Acq On : 21 Jul 2022 13:00
Operator : SY/MD
Sample : N3792-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN4

Quant Time: Jul 22 04:12:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 22 03:08:56 2022
Response via : Initial Calibration

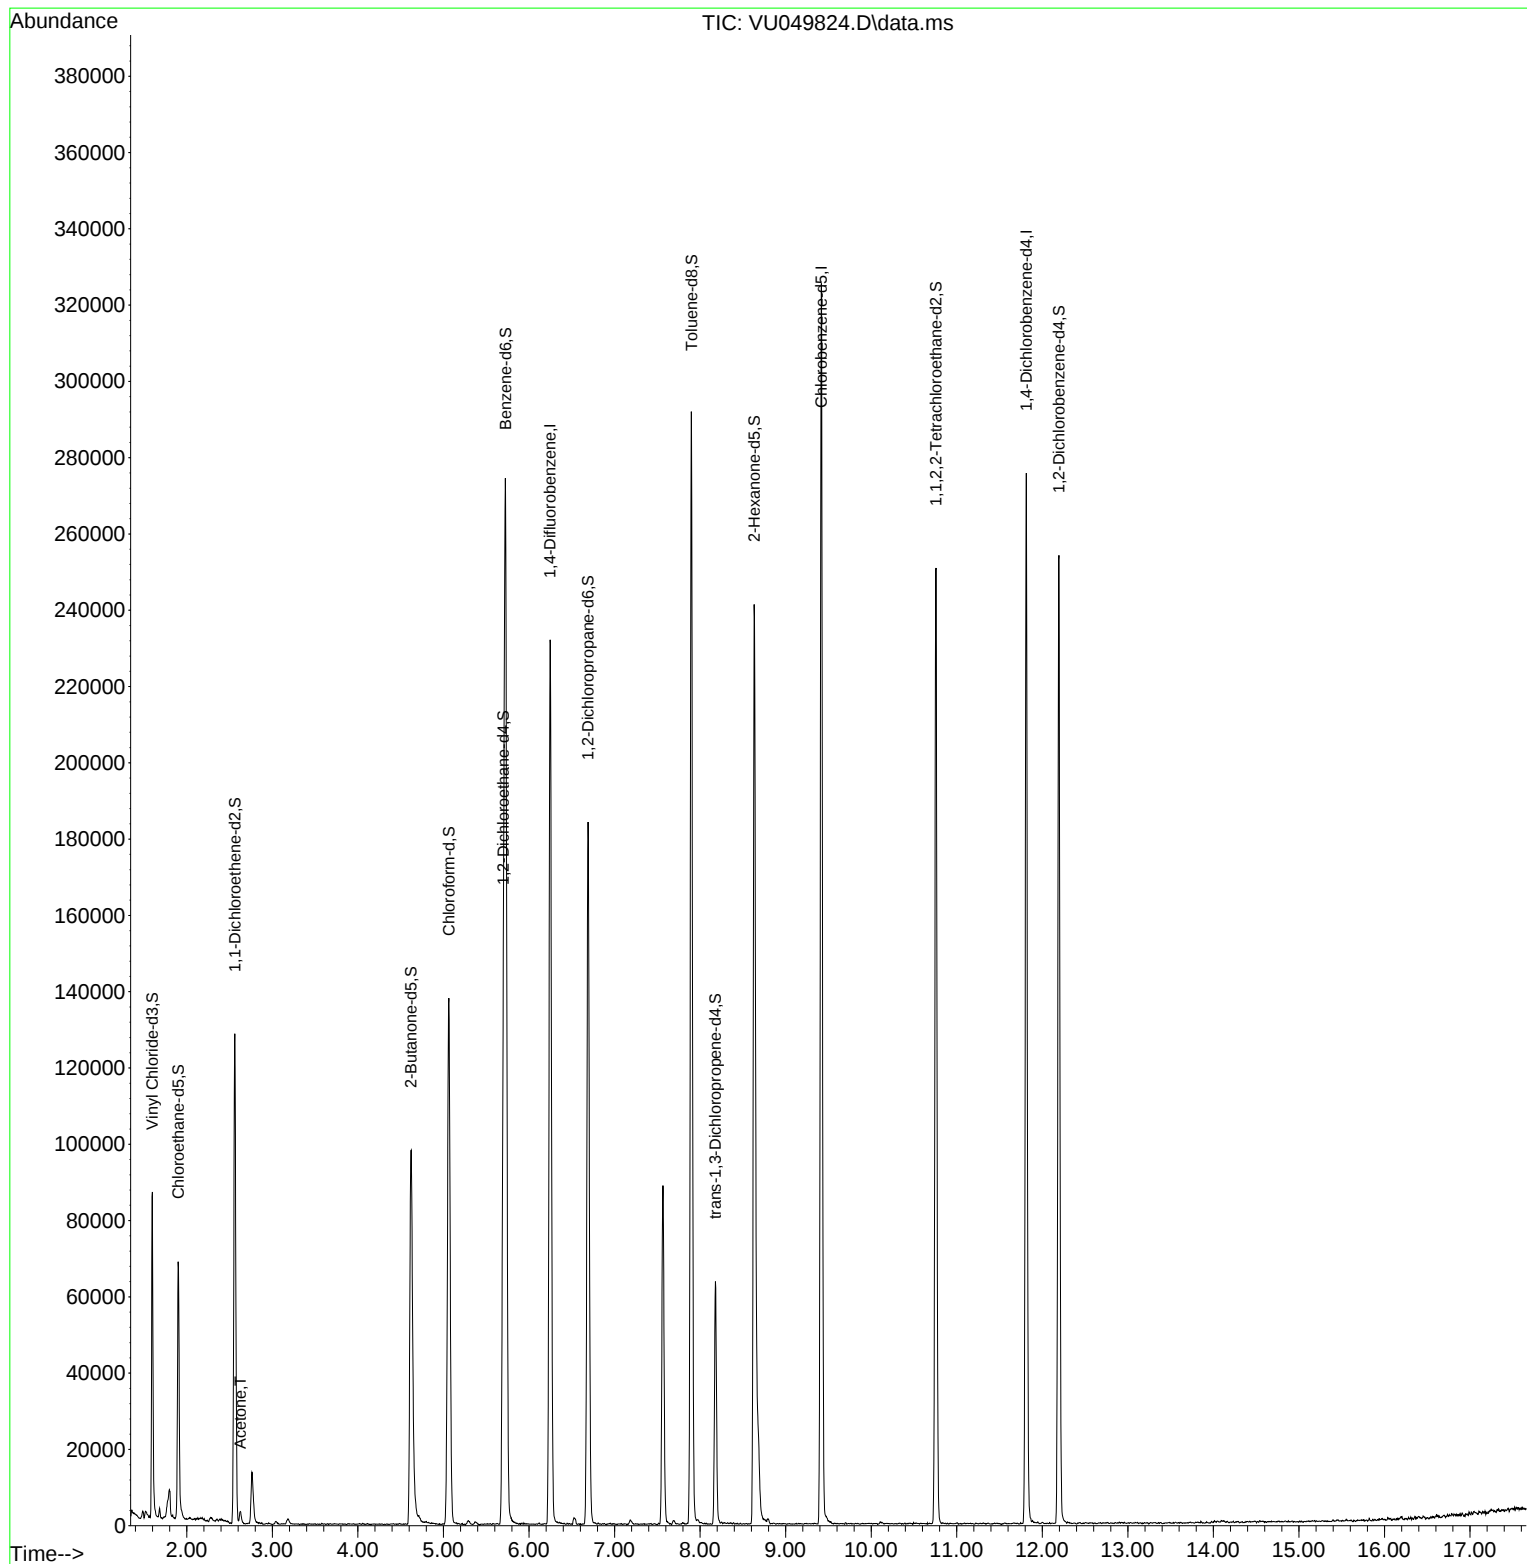

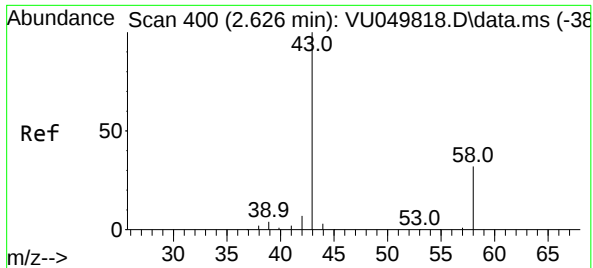

#13
 Acetone
 Concen: 2.897 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: VU049824.D
 Acq: 21 Jul 2022 13:00

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN4

Tgt Ion: 43 Resp: 3509
 Ion Ratio Lower Upper
 43 100
 58 31.7 0.0 61.4

