

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049828.D
 Acq On : 21 Jul 2022 14:35
 Operator : SY/MD
 Sample : N3792-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN0

Quant Time: Jul 22 04:13:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 22 03:08:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	174076	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	165439	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	66417	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	60547	41.223	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	82.440%	
7) Chloroethane-d5	1.900	69	48185	45.386	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	90.780%	
11) 1,1-Dichloroethene-d2	2.559	63	77936	30.040	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	60.080%	
21) 2-Butanone-d5	4.623	46	138936	110.809	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	110.810%	
24) Chloroform-d	5.063	84	127915	49.172	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.340%	
26) 1,2-Dichloroethane-d4	5.703	65	90607	51.463	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.920%	
32) Benzene-d6	5.726	84	230656	45.893	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.780%	
36) 1,2-Dichloropropane-d6	6.690	67	85031	50.299	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	100.600%	
41) Toluene-d8	7.899	98	186969	42.717	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	85.440%	
43) trans-1,3-Dichloroprop...	8.179	79	33205	46.619	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	93.240%	
47) 2-Hexanone-d5	8.632	63	71731	94.328	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	94.330%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	122616	51.837	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	103.680%	
66) 1,2-Dichlorobenzene-d4	12.195	152	62706	50.074	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.140%	
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	2902	2.435	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049828.D
Acq On : 21 Jul 2022 14:35
Operator : SY/MD
Sample : N3792-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN0

Quant Time: Jul 22 04:13:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 22 03:08:56 2022
Response via : Initial Calibration

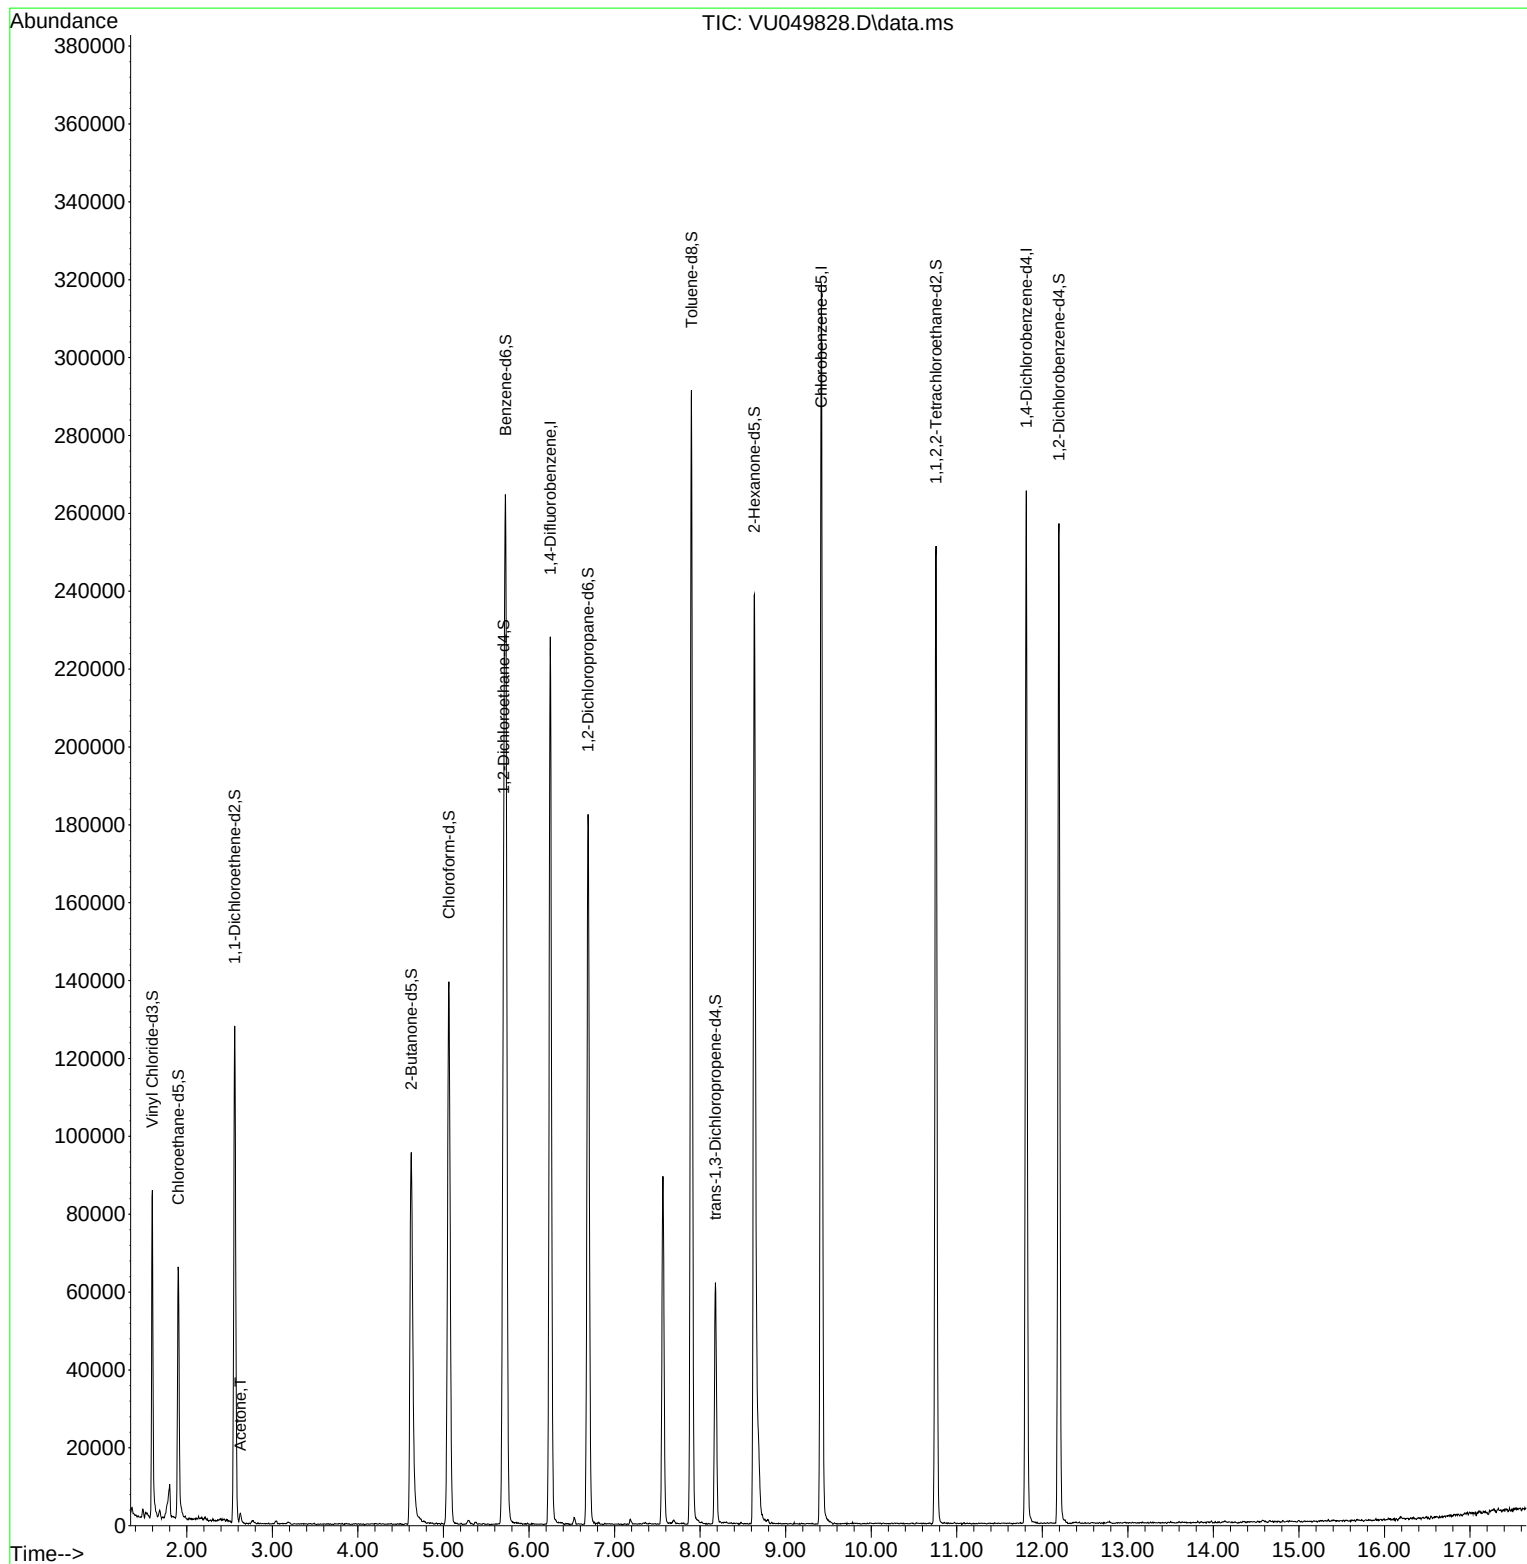

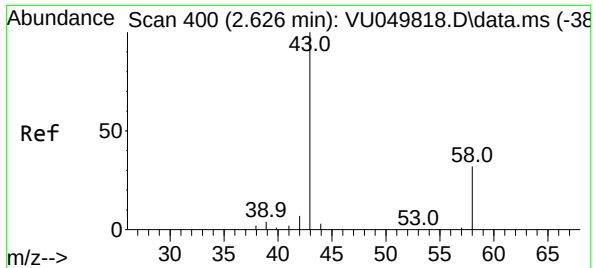

#13
 Acetone
 Concen: 2.435 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: VU049828.D
 Acq: 21 Jul 2022 14:35

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN0

Tgt Ion: 43 Resp: 2902
 Ion Ratio Lower Upper
 43 100
 58 32.5 0.0 61.4

