

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049824.D
 Acq On : 21 Jul 2022 13:00
 Operator : SY/MD
 Sample : N3792-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	98	rBV	85383	98441	13.36%	1.761%
2	1.681	103	106	112	rVB2	2594	2256	0.31%	0.040%
3	1.797	128	142	151	rBV6	7017	14493	1.97%	0.259%
4	1.900	166	174	199	rVB	67510	93864	12.74%	1.679%
5	2.276	285	291	294	rBV5	1092	1410	0.19%	0.025%
6	2.562	368	380	393	rBV	128372	208248	28.27%	3.726%
7	2.626	394	400	409	rVB2	2878	4392	0.60%	0.079%
8	2.761	432	442	458	rBV2	13456	25453	3.45%	0.455%
9	2.845	465	468	471	rBV3	303	203	0.03%	0.004%
10	2.957	500	503	505	rBV	277	138	0.02%	0.002%
11	3.044	516	530	536	rBV5	946	1903	0.26%	0.034%
12	3.182	564	573	584	rBV5	1310	2598	0.35%	0.046%
13	3.337	615	621	624	rBV2	269	290	0.04%	0.005%
14	3.356	624	627	629	rVV2	236	157	0.02%	0.003%
15	3.372	629	632	635	rVB2	187	129	0.02%	0.002%
16	3.433	647	651	654	rBV2	203	159	0.02%	0.003%
17	3.578	694	696	701	rVB	266	167	0.02%	0.003%
18	3.645	711	717	720	rVB	248	258	0.04%	0.005%
19	3.674	724	726	733	rVB	178	166	0.02%	0.003%
20	3.787	757	761	766	rBV2	174	235	0.03%	0.004%
21	3.883	787	791	793	rBV2	207	167	0.02%	0.003%
22	4.057	841	845	848	rBV	288	220	0.03%	0.004%
23	4.108	858	861	864	rBV2	215	141	0.02%	0.003%
24	4.141	868	871	875	rVB2	202	173	0.02%	0.003%
25	4.160	875	877	879	rBV	201	142	0.02%	0.003%
26	4.488	973	979	982	rBV2	233	264	0.04%	0.005%
27	4.552	996	999	1003	rBV	228	189	0.03%	0.003%
28	4.623	1008	1021	1046	rBV	98048	235000	31.90%	4.204%
29	4.864	1093	1096	1099	rBV2	260	157	0.02%	0.003%
30	4.919	1109	1113	1117	rBV2	147	125	0.02%	0.002%
31	4.954	1121	1124	1129	rBV2	219	139	0.02%	0.002%
32	5.063	1142	1158	1177	rBV	137881	300223	40.75%	5.371%
33	5.169	1188	1191	1193	rBV2	219	142	0.02%	0.003%
34	5.292	1218	1229	1232	rBV2	1207	2082	0.28%	0.037%
35	5.369	1245	1253	1264	rBV4	682	1330	0.18%	0.024%
36	5.443	1270	1276	1278	rBV2	250	300	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049824.D
 Acq On : 21 Jul 2022 13:00
 Operator : SY/MD
 Sample : N3792-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	5.578	1314	1318	1325	rBV2	291	335	0.05%	0.006%
38	5.723	1342	1363	1388	rBV2	274214	736713	100.00%	13.181%
39	5.893	1413	1416	1418	rVB2	263	142	0.02%	0.003%
40	5.919	1418	1424	1427	rBV2	360	302	0.04%	0.005%
41	5.951	1432	1434	1437	rVB2	244	135	0.02%	0.002%
42	6.118	1480	1486	1490	rBV3	359	351	0.05%	0.006%
43	6.247	1513	1526	1550	rBV	231809	441667	59.95%	7.902%
44	6.446	1585	1588	1592	rVB	309	196	0.03%	0.004%
45	6.526	1607	1613	1625	rBV5	1734	3228	0.44%	0.058%
46	6.690	1649	1664	1683	rBV	184072	352968	47.91%	6.315%
47	6.809	1698	1701	1705	rVB2	331	249	0.03%	0.004%
48	6.857	1712	1716	1720	rBV	221	217	0.03%	0.004%
49	6.880	1720	1723	1730	rVB2	365	386	0.05%	0.007%
50	6.948	1742	1744	1747	rVV2	322	180	0.02%	0.003%
51	6.993	1755	1758	1762	rVB	209	143	0.02%	0.003%
52	7.076	1781	1784	1790	rVB2	225	169	0.02%	0.003%
53	7.153	1805	1808	1811	rBV2	226	205	0.03%	0.004%
54	7.185	1811	1818	1829	rVV3	1193	2262	0.31%	0.040%
55	7.465	1899	1905	1912	rVB2	218	311	0.04%	0.006%
56	7.513	1916	1920	1924	rBV	423	395	0.05%	0.007%
57	7.565	1924	1936	1960	rVB	88768	156856	21.29%	2.806%
58	7.687	1967	1974	1976	rBV2	1117	1276	0.17%	0.023%
59	7.796	2002	2008	2011	rBV2	476	467	0.06%	0.008%
60	7.896	2027	2039	2058	rBV	291447	498102	67.61%	8.912%
61	8.073	2091	2094	2097	rVB2	304	218	0.03%	0.004%
62	8.121	2106	2109	2114	rVB2	186	138	0.02%	0.002%
63	8.179	2115	2127	2145	rBV2	63612	102946	13.97%	1.842%
64	8.391	2189	2193	2197	rVB2	377	317	0.04%	0.006%
65	8.468	2215	2217	2223	rVB2	280	208	0.03%	0.004%
66	8.565	2244	2247	2251	rBV	164	131	0.02%	0.002%
67	8.632	2256	2268	2301	rBV2	240963	491855	66.76%	8.800%
68	8.793	2313	2318	2326	rVB5	1363	2083	0.28%	0.037%
69	8.902	2347	2352	2356	rBV2	234	255	0.03%	0.005%
70	9.333	2483	2486	2488	rBV	213	132	0.02%	0.002%
71	9.417	2499	2512	2537	rBV	325215	530738	72.04%	9.495%
72	9.568	2556	2559	2562	rBV3	210	164	0.02%	0.003%
73	9.700	2597	2600	2604	rBV3	448	380	0.05%	0.007%
74	10.105	2723	2726	2730	rVV	653	615	0.08%	0.011%
75	10.124	2730	2732	2738	rVB2	486	416	0.06%	0.007%
76	10.369	2804	2808	2811	rBV	210	220	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049824.D
 Acq On : 21 Jul 2022 13:00
 Operator : SY/MD
 Sample : N3792-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.394	2812	2816	2820	rVB2	303	255	0.03%	0.005%
78	10.420	2820	2824	2827	rBV2	246	217	0.03%	0.004%
79	10.494	2844	2847	2851	rBV2	465	359	0.05%	0.006%
80	10.581	2869	2874	2877	rBV2	217	243	0.03%	0.004%
81	10.758	2915	2929	2949	rVB	250556	404590	54.92%	7.239%
82	10.832	2949	2952	2954	rBV	214	152	0.02%	0.003%
83	11.224	3070	3074	3083	rBV2	277	366	0.05%	0.007%
84	11.365	3110	3118	3128	rBV2	316	563	0.08%	0.010%
85	11.426	3134	3137	3139	rBV2	167	126	0.02%	0.002%
86	11.533	3166	3170	3172	rBV	229	181	0.02%	0.003%
87	11.558	3172	3178	3181	rBV2	282	342	0.05%	0.006%
88	11.748	3233	3237	3240	rBV2	351	214	0.03%	0.004%
89	11.812	3244	3257	3276	rVV	275324	436406	59.24%	7.808%
90	12.086	3339	3342	3346	rVB	337	221	0.03%	0.004%
91	12.195	3363	3376	3404	rVB	253777	418904	56.86%	7.495%
92	12.478	3461	3464	3467	rBV2	205	132	0.02%	0.002%
93	12.957	3611	3613	3622	rVB	270	224	0.03%	0.004%
94	13.169	3676	3679	3681	rVB	236	128	0.02%	0.002%
95	13.266	3703	3709	3714	rBV2	374	558	0.08%	0.010%
96	13.378	3741	3744	3745	rBV	229	141	0.02%	0.003%
97	13.854	3890	3892	3898	rVB2	483	349	0.05%	0.006%
98	13.976	3928	3930	3933	rBV	303	177	0.02%	0.003%
99	14.012	3939	3941	3946	rVB	383	236	0.03%	0.004%
100	16.037	4569	4571	4575	rBV	648	460	0.06%	0.008%




Sum of corrected areas: 5589369

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049824.D
Acq On : 21 Jul 2022 13:00
Operator : SY/MD
Sample : N3792-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

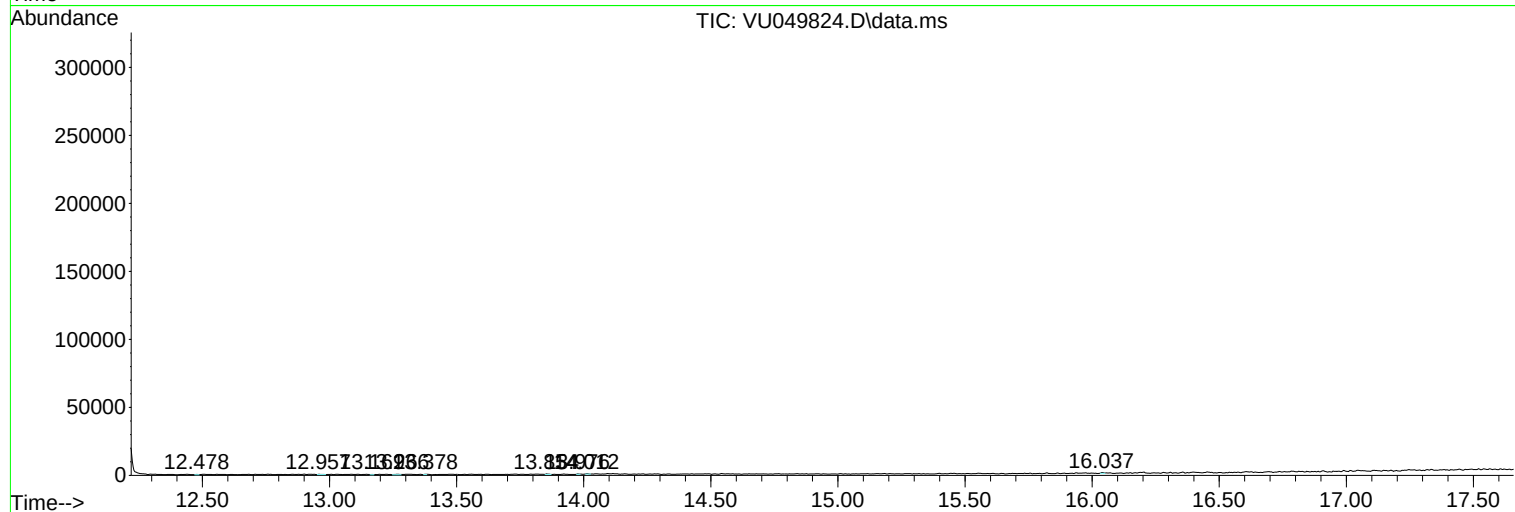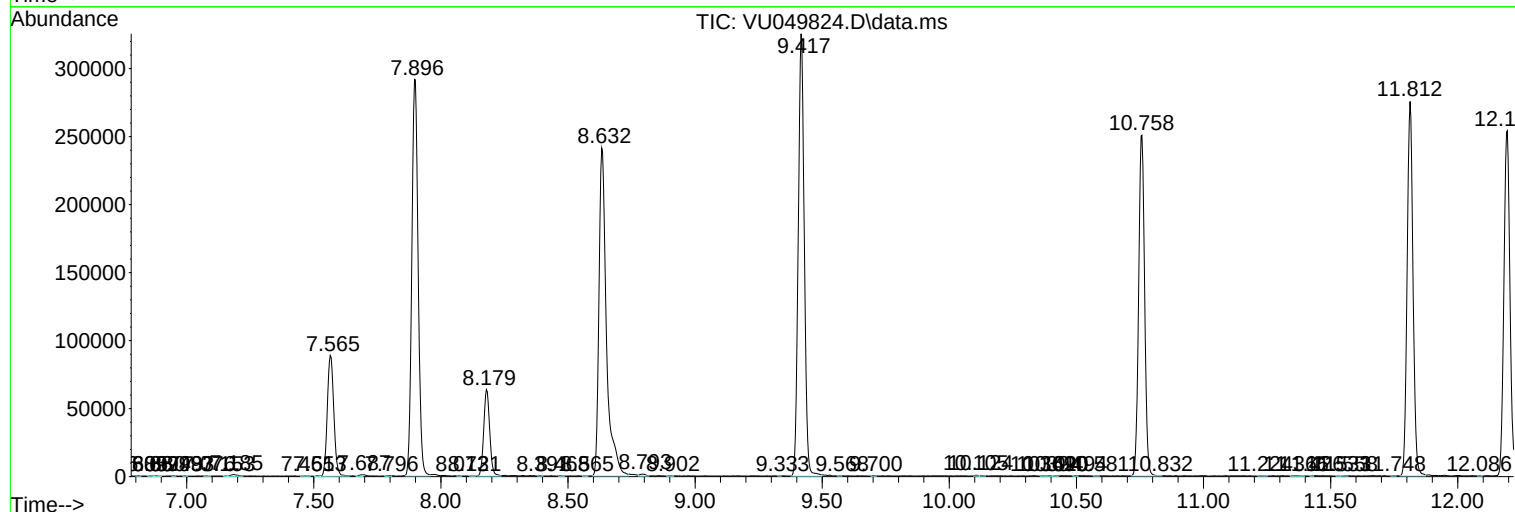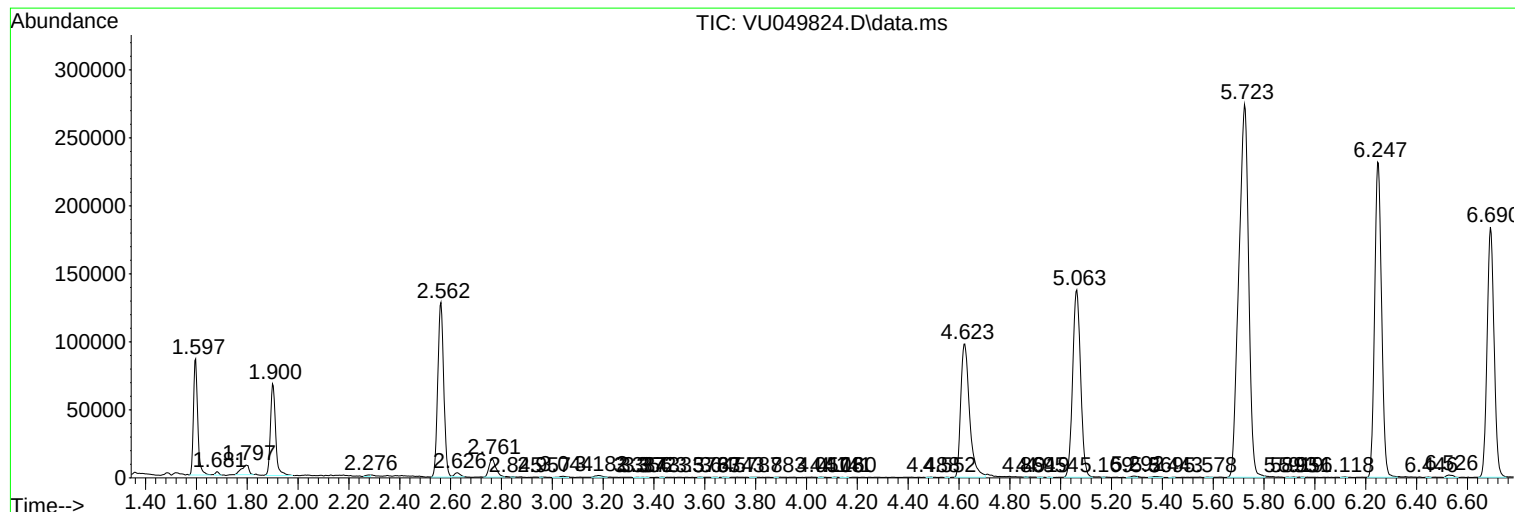

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049824.D
Acq On : 21 Jul 2022 13:00
Operator : SY/MD
Sample : N3792-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.761	2.88 ug/L	25453	1,4-Difluorobenzene	6.247

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
2			2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	9
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

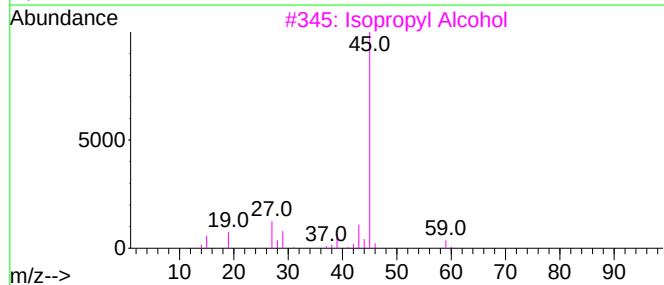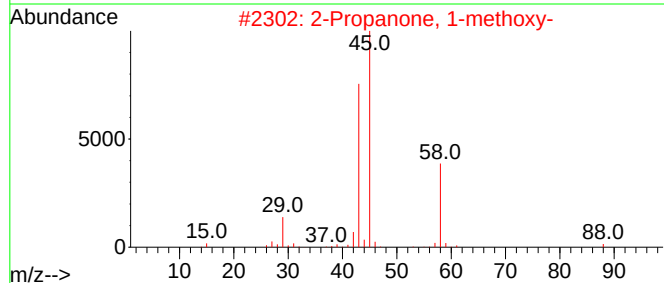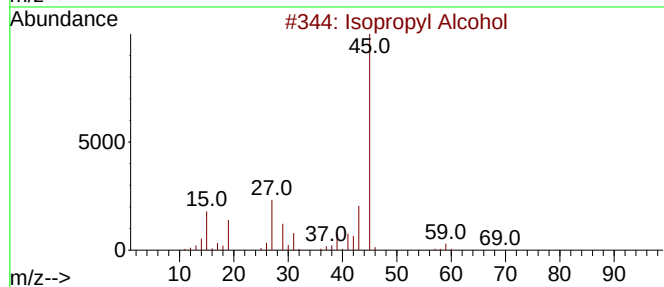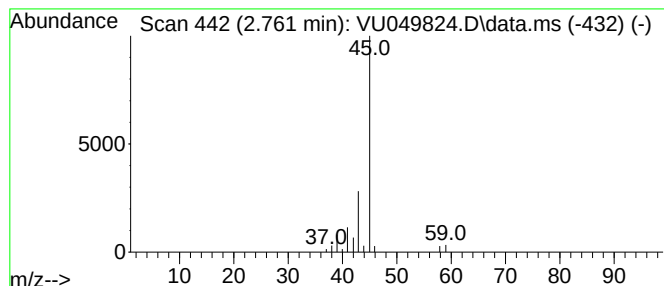

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049824.D
Acq On : 21 Jul 2022 13:00
Operator : SY/MD
Sample : N3792-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	2.761	2.9	ug/L	25453	1	6.247	441667	50.0