

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049825.D
 Acq On : 21 Jul 2022 13:24
 Operator : SY/MD
 Sample : N3792-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.517	52	55	65	rBV3	1207	1847	0.25%	0.033%
2	1.597	73	80	95	rVB	88815	97180	13.06%	1.748%
3	1.900	165	174	184	rBV	67982	89913	12.08%	1.617%
4	2.282	290	293	298	rVB3	778	698	0.09%	0.013%
5	2.327	304	307	311	rBV2	370	220	0.03%	0.004%
6	2.388	324	326	329	rBV2	537	376	0.05%	0.007%
7	2.562	368	380	393	rBV	128693	208903	28.07%	3.758%
8	2.626	396	400	413	rVB2	1859	3076	0.41%	0.055%
9	2.694	418	421	424	rVB2	371	268	0.04%	0.005%
10	2.768	433	444	456	rBV2	8393	17242	2.32%	0.310%
11	2.861	469	473	479	rVB3	561	672	0.09%	0.012%
12	2.900	479	485	488	rBV2	486	621	0.08%	0.011%
13	2.919	489	491	497	rVB	283	158	0.02%	0.003%
14	2.957	500	503	506	rVB2	398	234	0.03%	0.004%
15	2.977	506	509	514	rVB2	213	193	0.03%	0.003%
16	3.006	514	518	523	rVB2	173	186	0.02%	0.003%
17	3.038	523	528	530	rBV3	673	632	0.08%	0.011%
18	3.179	566	572	574	rBV2	682	746	0.10%	0.013%
19	3.813	765	769	772	rBV2	235	200	0.03%	0.004%
20	4.060	843	846	852	rVB2	199	224	0.03%	0.004%
21	4.298	915	920	924	rBV2	228	241	0.03%	0.004%
22	4.414	950	956	958	rBV2	239	280	0.04%	0.005%
23	4.456	965	969	971	rBV2	222	159	0.02%	0.003%
24	4.620	1008	1020	1050	rBV	96558	235819	31.68%	4.242%
25	4.864	1094	1096	1101	rBV2	225	151	0.02%	0.003%
26	5.063	1137	1158	1176	rBV	139164	304920	40.97%	5.485%
27	5.285	1221	1227	1230	rBV4	734	801	0.11%	0.014%
28	5.446	1272	1277	1282	rBV2	326	368	0.05%	0.007%
29	5.591	1318	1322	1325	rBV2	239	211	0.03%	0.004%
30	5.723	1341	1363	1385	rBV2	266554	744267	100.00%	13.388%
31	5.954	1430	1435	1437	rBV2	301	259	0.03%	0.005%
32	6.076	1467	1473	1476	rBV2	231	235	0.03%	0.004%
33	6.250	1513	1527	1551	rVV	228801	431391	57.96%	7.760%
34	6.452	1588	1590	1596	rVB	430	376	0.05%	0.007%
35	6.481	1596	1599	1602	rBV	377	327	0.04%	0.006%
36	6.498	1602	1604	1606	rVV2	280	174	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049825.D
 Acq On : 21 Jul 2022 13:24
 Operator : SY/MD
 Sample : N3792-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.533	1606	1615	1625	rVB5	1725	3225	0.43%	0.058%
38	6.629	1641	1645	1649	rBV	240	218	0.03%	0.004%
39	6.690	1650	1664	1684	rVV	185288	353887	47.55%	6.366%
40	6.809	1697	1701	1707	rVB2	293	303	0.04%	0.005%
41	7.070	1772	1782	1789	rBV2	232	399	0.05%	0.007%
42	7.186	1810	1818	1825	rVV6	1398	2364	0.32%	0.043%
43	7.350	1866	1869	1876	rBV2	143	147	0.02%	0.003%
44	7.401	1880	1885	1890	rVB	215	199	0.03%	0.004%
45	7.565	1924	1936	1955	rBV	90946	159256	21.40%	2.865%
46	7.694	1968	1976	1979	rVV4	874	1010	0.14%	0.018%
47	7.751	1988	1994	1996	rBV	260	207	0.03%	0.004%
48	7.793	2003	2007	2015	rVB2	543	897	0.12%	0.016%
49	7.899	2025	2040	2059	rBV	288238	499221	67.08%	8.980%
50	8.018	2075	2077	2089	rVB4	430	468	0.06%	0.008%
51	8.179	2115	2127	2145	rBV2	61739	104455	14.03%	1.879%
52	8.359	2179	2183	2185	rBV2	317	272	0.04%	0.005%
53	8.514	2227	2231	2235	rVB	290	268	0.04%	0.005%
54	8.568	2244	2248	2254	rBV	244	210	0.03%	0.004%
55	8.632	2255	2268	2299	rBV2	239131	490879	65.95%	8.830%
56	8.784	2313	2315	2319	rBV3	424	360	0.05%	0.006%
57	8.996	2377	2381	2386	rBV2	234	186	0.02%	0.003%
58	9.044	2392	2396	2398	rBV	217	176	0.02%	0.003%
59	9.102	2410	2414	2417	rBV2	190	139	0.02%	0.003%
60	9.150	2423	2429	2435	rBV2	226	317	0.04%	0.006%
61	9.417	2499	2512	2535	rBV	317332	523154	70.29%	9.410%
62	9.626	2574	2577	2581	rVB	316	214	0.03%	0.004%
63	9.719	2604	2606	2612	rVB2	241	178	0.02%	0.003%
64	9.796	2626	2630	2632	rBV	208	150	0.02%	0.003%
65	9.976	2683	2686	2691	rVB2	289	213	0.03%	0.004%
66	10.304	2784	2788	2791	rBV2	194	175	0.02%	0.003%
67	10.346	2798	2801	2804	rVV	198	138	0.02%	0.002%
68	10.427	2822	2826	2833	rVB	308	323	0.04%	0.006%
69	10.481	2839	2843	2846	rVB2	206	154	0.02%	0.003%
70	10.529	2855	2858	2862	rVB2	191	157	0.02%	0.003%
71	10.758	2916	2929	2949	rBV	255227	411683	55.31%	7.405%
72	11.054	3016	3021	3024	rBV2	222	236	0.03%	0.004%
73	11.195	3062	3065	3069	rVB2	241	146	0.02%	0.003%
74	11.382	3120	3123	3126	rVB2	177	147	0.02%	0.003%
75	11.407	3126	3131	3134	rBV2	224	231	0.03%	0.004%
76	11.558	3173	3178	3182	rBV2	205	235	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049825.D
 Acq On : 21 Jul 2022 13:24
 Operator : SY/MD
 Sample : N3792-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.745	3232	3236	3238	rBV2	465	322	0.04%	0.006%
78	11.812	3245	3257	3276	rBV	268067	426451	57.30%	7.671%
79	11.938	3293	3296	3299	rBV3	189	155	0.02%	0.003%
80	12.195	3363	3376	3401	rBV	256877	424294	57.01%	7.632%
81	12.291	3401	3406	3409	rVV3	558	490	0.07%	0.009%
82	12.359	3424	3427	3432	rVB	234	209	0.03%	0.004%
83	12.388	3432	3436	3439	rBV	299	243	0.03%	0.004%
84	12.436	3447	3451	3456	rBV2	394	392	0.05%	0.007%
85	12.533	3478	3481	3487	rBV2	347	316	0.04%	0.006%
86	12.626	3508	3510	3515	rBV2	191	139	0.02%	0.003%
87	12.825	3569	3572	3577	rVB2	357	327	0.04%	0.006%
88	12.864	3577	3584	3590	rBV2	558	932	0.13%	0.017%
89	13.185	3681	3684	3686	rBV2	203	149	0.02%	0.003%
90	13.317	3722	3725	3729	rVB2	535	347	0.05%	0.006%
91	13.590	3807	3810	3814	rBV2	373	304	0.04%	0.005%
92	13.680	3835	3838	3841	rBV	234	154	0.02%	0.003%
93	13.697	3841	3843	3847	rVV2	242	157	0.02%	0.003%
94	14.044	3946	3951	3954	rBV3	438	424	0.06%	0.008%
95	14.391	4055	4059	4062	rBV2	371	371	0.05%	0.007%
96	14.574	4112	4116	4124	rBV3	785	1309	0.18%	0.024%
97	15.012	4250	4252	4254	rBV2	419	273	0.04%	0.005%
98	15.758	4483	4484	4489	rVB2	458	274	0.04%	0.005%
99	16.063	4577	4579	4584	rBV2	527	388	0.05%	0.007%
100	16.536	4724	4726	4732	rBV4	786	685	0.09%	0.012%




Sum of corrected areas: 5559270

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049825.D
Acq On : 21 Jul 2022 13:24
Operator : SY/MD
Sample : N3792-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

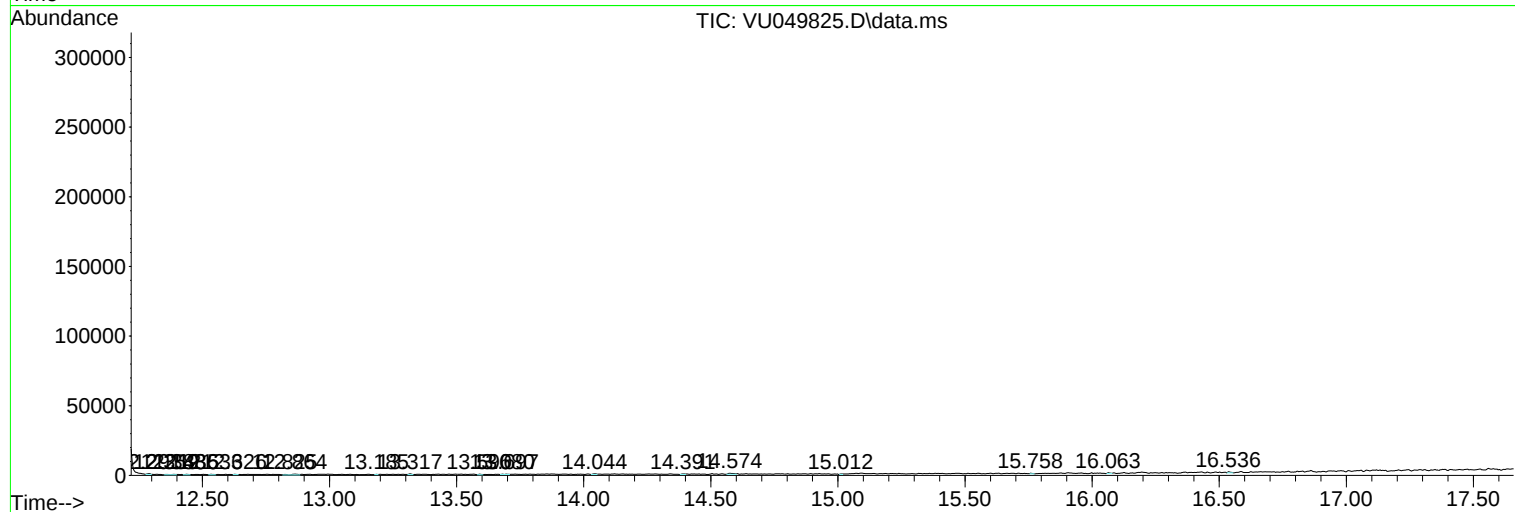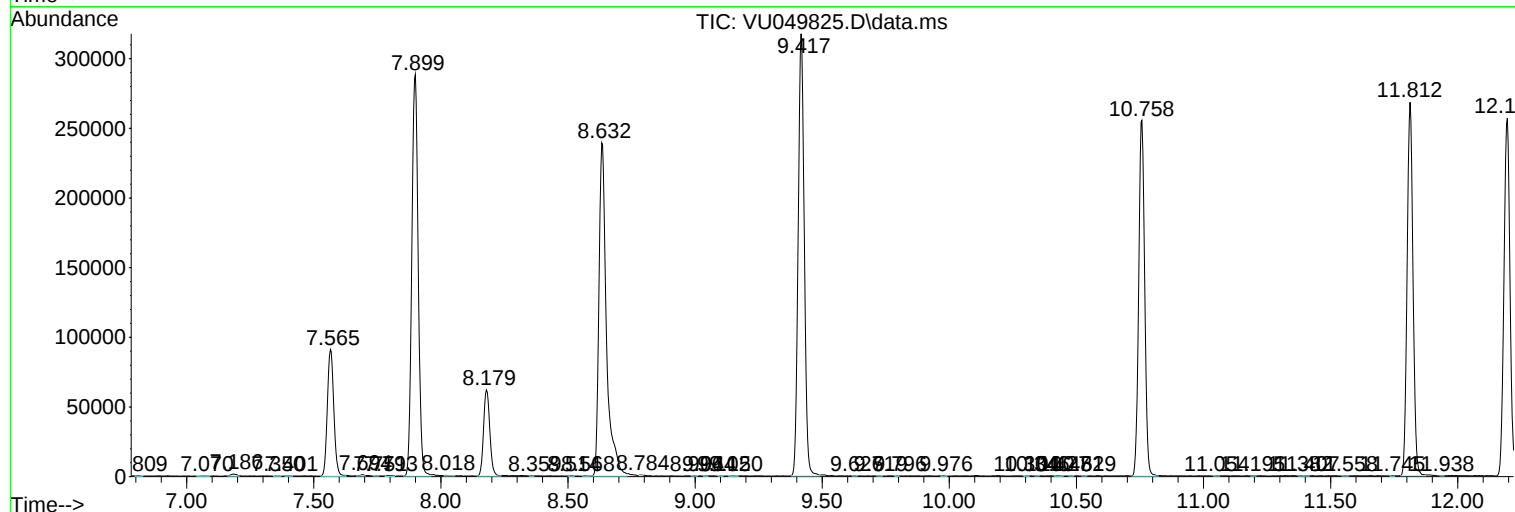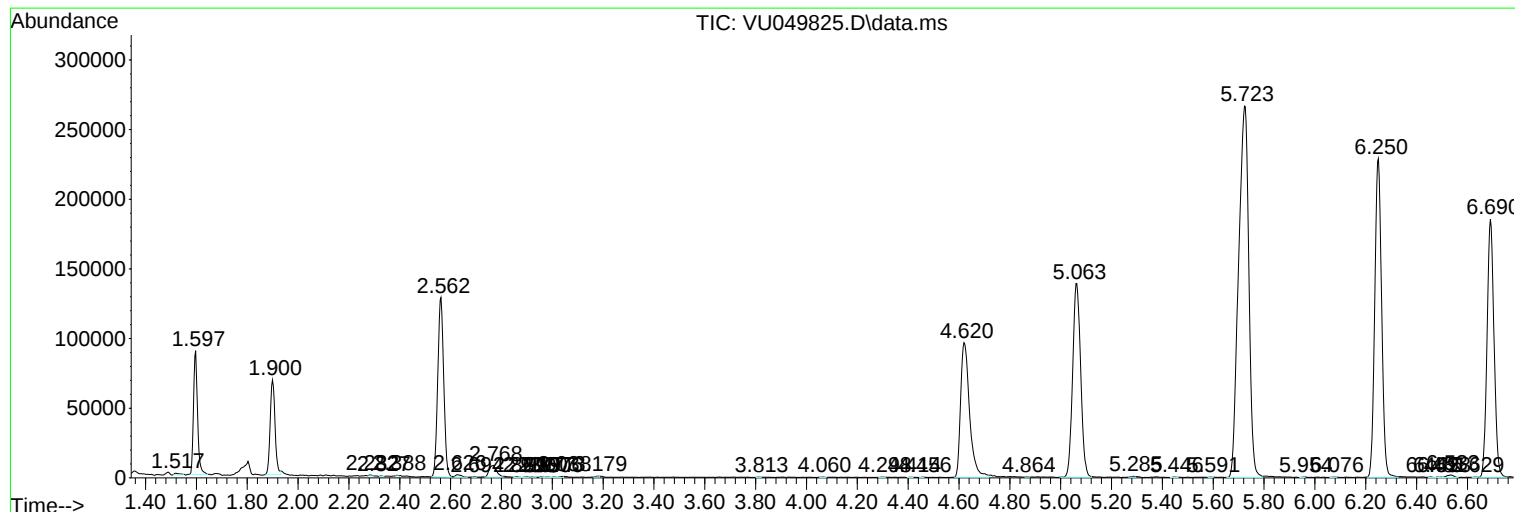

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049825.D
Acq On : 21 Jul 2022 13:24
Operator : SY/MD
Sample : N3792-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049825.D
Acq On : 21 Jul 2022 13:24
Operator : SY/MD
Sample : N3792-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------