

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049826.D
 Acq On : 21 Jul 2022 13:48
 Operator : SY/MD
 Sample : N3792-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M

Title : VOC Analysis

Signal : TIC: VU049826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	41	46	52	rBV3	1750	2029	0.26%	0.036%
2	1.597	72	80	100	rBV	89490	103867	13.51%	1.817%
3	1.861	160	162	165	rBV2	674	525	0.07%	0.009%
4	1.903	166	175	196	rVB	69973	97241	12.65%	1.701%
5	2.276	288	291	295	rBV3	563	398	0.05%	0.007%
6	2.375	320	322	324	rBV3	322	192	0.02%	0.003%
7	2.420	334	336	337	rBV	485	211	0.03%	0.004%
8	2.562	367	380	395	rBV	135063	218318	28.40%	3.820%
9	2.623	397	399	408	rVB3	1222	1583	0.21%	0.028%
10	2.694	418	421	425	rBV2	233	169	0.02%	0.003%
11	2.758	438	441	442	rBV	360	217	0.03%	0.004%
12	2.964	502	505	508	rBV2	292	272	0.04%	0.005%
13	3.038	523	528	536	rVV5	926	1411	0.18%	0.025%
14	3.166	565	568	571	rBV2	506	445	0.06%	0.008%
15	3.279	601	603	606	rBV	335	187	0.02%	0.003%
16	3.546	680	686	689	rBV2	178	196	0.03%	0.003%
17	3.584	695	698	702	rBV	172	170	0.02%	0.003%
18	3.629	709	712	716	rVB2	256	215	0.03%	0.004%
19	3.655	716	720	722	rBV2	241	189	0.02%	0.003%
20	3.674	723	726	730	rVB	204	162	0.02%	0.003%
21	3.867	778	786	790	rBV3	902	1275	0.17%	0.022%
22	4.041	837	840	849	rVB2	172	202	0.03%	0.004%
23	4.150	869	874	881	rVB2	287	324	0.04%	0.006%
24	4.192	882	887	888	rBV	207	165	0.02%	0.003%
25	4.247	899	904	908	rBV	260	264	0.03%	0.005%
26	4.362	934	940	943	rBV	284	230	0.03%	0.004%
27	4.533	988	993	999	rVB2	234	326	0.04%	0.006%
28	4.571	999	1005	1007	rBV2	174	176	0.02%	0.003%
29	4.623	1007	1021	1057	rBV	101733	248829	32.37%	4.354%
30	4.841	1087	1089	1093	rVB	277	163	0.02%	0.003%
31	4.864	1093	1096	1099	rBV	258	214	0.03%	0.004%
32	4.931	1114	1117	1121	rBV3	268	207	0.03%	0.004%
33	5.063	1141	1158	1183	rVV	144196	317236	41.27%	5.551%
34	5.288	1221	1228	1237	rVB5	1110	2015	0.26%	0.035%
35	5.343	1237	1245	1249	rBV2	258	258	0.03%	0.005%
36	5.382	1249	1257	1262	rBV4	657	1045	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049826.D
 Acq On : 21 Jul 2022 13:48
 Operator : SY/MD
 Sample : N3792-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	5.726	1343	1364	1387	rBV2	279714	768695	100.00%	13.450%
38	5.838	1396	1399	1409	rVB3	409	584	0.08%	0.010%
39	5.912	1417	1422	1426	rVV2	232	241	0.03%	0.004%
40	5.973	1438	1441	1446	rBV2	304	264	0.03%	0.005%
41	6.025	1452	1457	1464	rVB	254	333	0.04%	0.006%
42	6.063	1464	1469	1472	rBV2	203	181	0.02%	0.003%
43	6.111	1481	1484	1488	rVB	270	216	0.03%	0.004%
44	6.179	1501	1505	1508	rBV2	227	207	0.03%	0.004%
45	6.250	1513	1527	1546	rBV	228234	434667	56.55%	7.605%
46	6.536	1607	1616	1622	rVB4	1740	3008	0.39%	0.053%
47	6.591	1630	1633	1636	rBV2	242	197	0.03%	0.003%
48	6.690	1651	1664	1684	rBV	189769	367090	47.75%	6.423%
49	7.031	1766	1770	1777	rBV2	250	290	0.04%	0.005%
50	7.185	1810	1818	1831	rVB3	1165	2138	0.28%	0.037%
51	7.369	1872	1875	1877	rBV2	266	209	0.03%	0.004%
52	7.565	1924	1936	1954	rVV	93120	162989	21.20%	2.852%
53	7.690	1970	1975	1985	rVB3	908	1414	0.18%	0.025%
54	7.787	2003	2005	2008	rVV3	306	210	0.03%	0.004%
55	7.806	2008	2011	2014	rVV2	245	159	0.02%	0.003%
56	7.899	2026	2040	2057	rBV	300399	519937	67.64%	9.097%
57	7.963	2057	2060	2072	rVB3	1275	2030	0.26%	0.036%
58	8.089	2094	2099	2100	rBV2	261	214	0.03%	0.004%
59	8.134	2108	2113	2116	rBV2	207	234	0.03%	0.004%
60	8.179	2116	2127	2142	rBV2	64264	109206	14.21%	1.911%
61	8.378	2184	2189	2193	rVB3	457	463	0.06%	0.008%
62	8.436	2205	2207	2215	rVB2	307	354	0.05%	0.006%
63	8.635	2256	2269	2311	rBV3	250845	516264	67.16%	9.033%
64	8.838	2330	2332	2336	rVB2	403	204	0.03%	0.004%
65	8.999	2378	2382	2383	rBV	213	160	0.02%	0.003%
66	9.166	2429	2434	2437	rBV2	213	204	0.03%	0.004%
67	9.304	2473	2477	2482	rBV2	271	280	0.04%	0.005%
68	9.417	2500	2512	2530	rBV	312582	521943	67.90%	9.133%
69	9.568	2554	2559	2563	rVB3	472	472	0.06%	0.008%
70	9.645	2580	2583	2587	rBV2	263	246	0.03%	0.004%
71	9.893	2657	2660	2666	rBV2	201	161	0.02%	0.003%
72	10.102	2720	2725	2727	rBV2	396	295	0.04%	0.005%
73	10.352	2800	2803	2807	rVV2	238	197	0.03%	0.003%
74	10.497	2845	2848	2852	rBV2	198	202	0.03%	0.004%
75	10.619	2882	2886	2889	rBV	372	358	0.05%	0.006%
76	10.664	2897	2900	2906	rVB	206	170	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049826.D
 Acq On : 21 Jul 2022 13:48
 Operator : SY/MD
 Sample : N3792-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.758	2916	2929	2953	rVV	262508	425001	55.29%	7.436%
78	10.870	2958	2964	2968	rBV2	285	371	0.05%	0.006%
79	10.909	2972	2976	2979	rBV2	325	316	0.04%	0.006%
80	11.008	3004	3007	3011	rVB	338	243	0.03%	0.004%
81	11.098	3032	3035	3039	rVB2	255	161	0.02%	0.003%
82	11.166	3053	3056	3059	rBV2	244	167	0.02%	0.003%
83	11.745	3234	3236	3241	rVB	314	229	0.03%	0.004%
84	11.812	3245	3257	3274	rBV	271529	428648	55.76%	7.500%
85	12.060	3331	3334	3338	rBV	352	271	0.04%	0.005%
86	12.082	3338	3341	3345	rVB3	360	277	0.04%	0.005%
87	12.195	3363	3376	3397	rBV	269254	436842	56.83%	7.644%
88	13.012	3627	3630	3635	rBV2	287	258	0.03%	0.005%
89	13.201	3686	3689	3692	rBV	414	309	0.04%	0.005%
90	13.240	3698	3701	3704	rBV2	396	271	0.04%	0.005%
91	13.407	3747	3753	3756	rBV2	474	519	0.07%	0.009%
92	13.465	3769	3771	3775	rBV	255	184	0.02%	0.003%
93	13.610	3810	3816	3825	rBV2	407	780	0.10%	0.014%
94	13.851	3889	3891	3897	rVB2	507	479	0.06%	0.008%
95	14.102	3966	3969	3974	rBV3	439	404	0.05%	0.007%
96	14.143	3980	3982	3984	rBV2	291	218	0.03%	0.004%
97	14.317	4033	4036	4042	rBV2	373	307	0.04%	0.005%
98	14.458	4077	4080	4087	rVB2	441	499	0.06%	0.009%
99	15.777	4487	4490	4493	rBV	510	472	0.06%	0.008%
100	16.146	4603	4605	4608	rBV2	496	361	0.05%	0.006%




Sum of corrected areas: 5715199

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049826.D
Acq On : 21 Jul 2022 13:48
Operator : SY/MD
Sample : N3792-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

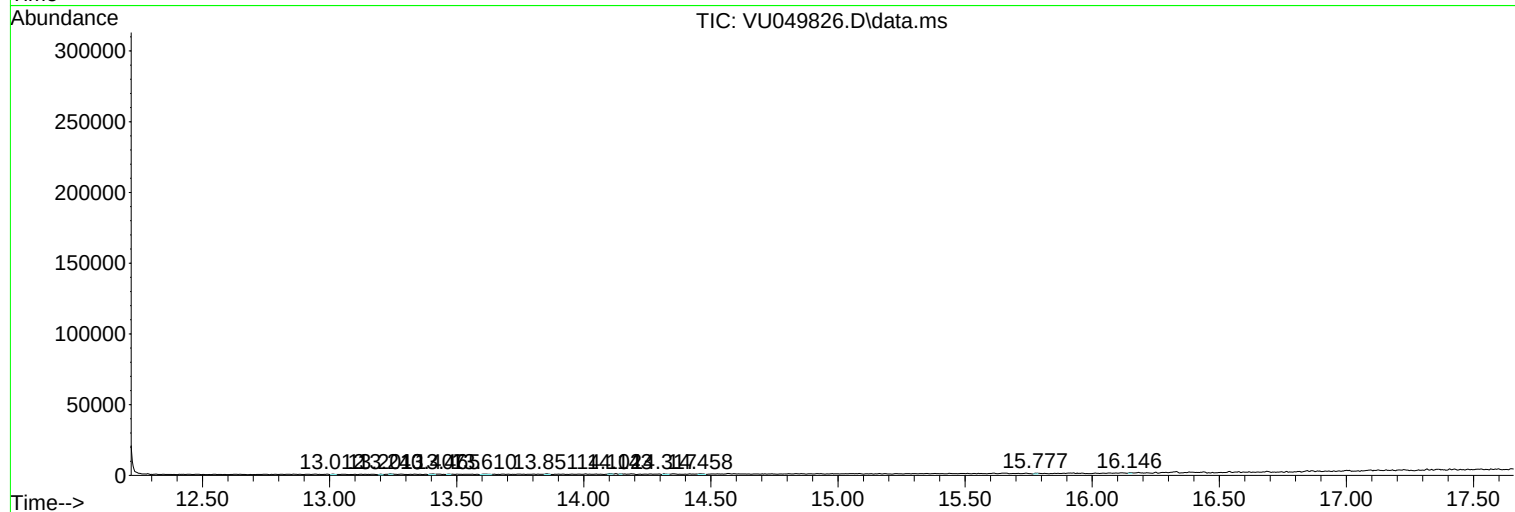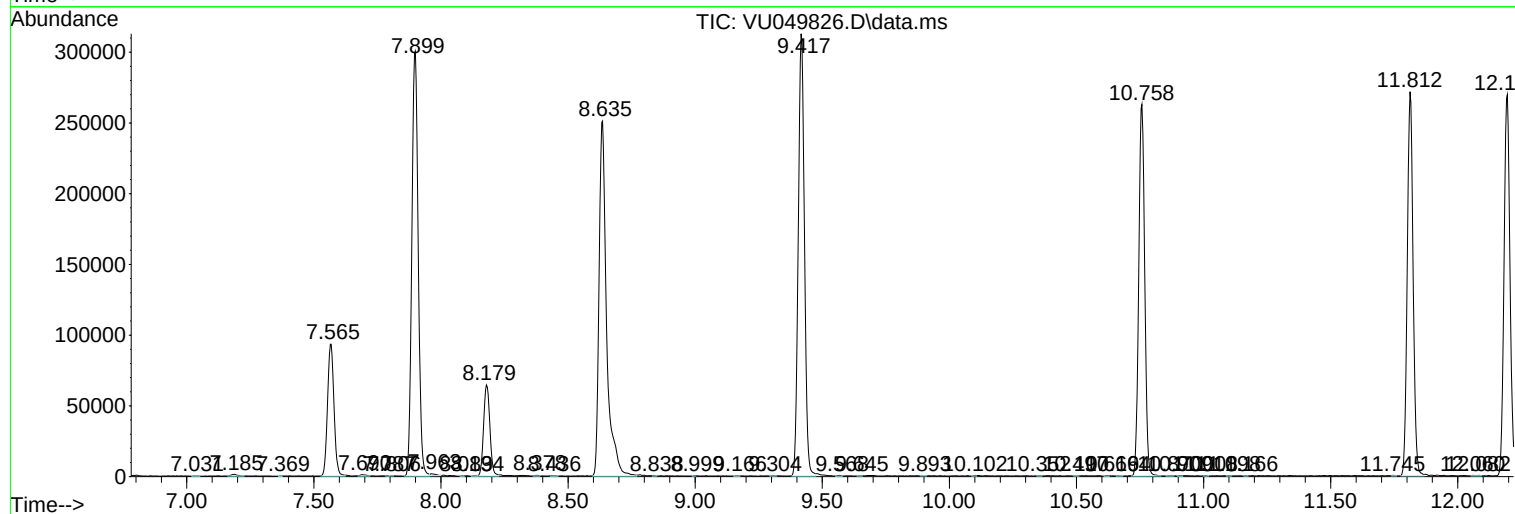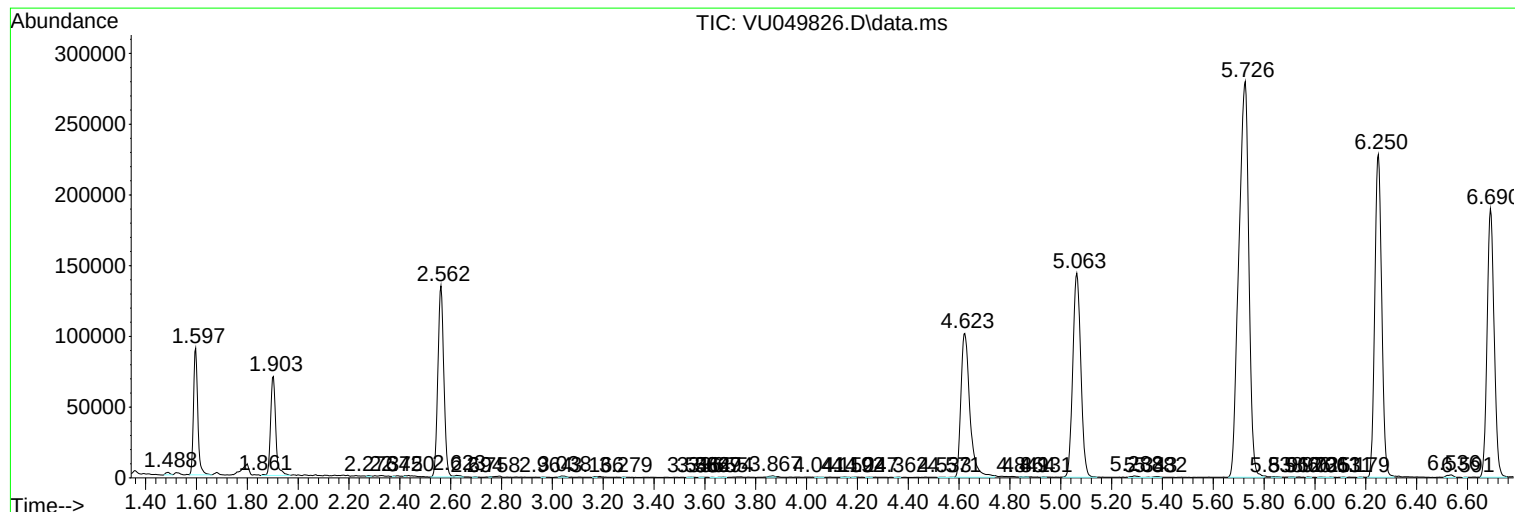

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049826.D
Acq On : 21 Jul 2022 13:48
Operator : SY/MD
Sample : N3792-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049826.D
Acq On : 21 Jul 2022 13:48
Operator : SY/MD
Sample : N3792-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc