

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049837.D
 Acq On : 21 Jul 2022 18:34
 Operator : SY/MD
 Sample : N3792-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rBV	87055	96950	12.70%	1.678%
2	1.803	126	144	152	rBV9	8675	18137	2.38%	0.314%
3	1.900	166	174	190	rBV	69335	92608	12.13%	1.603%
4	2.507	361	363	365	rBV	316	173	0.02%	0.003%
5	2.559	367	379	394	rVV	132349	214088	28.04%	3.706%
6	2.771	442	445	448	rVV3	309	267	0.03%	0.005%
7	2.790	448	451	456	rVB3	701	572	0.07%	0.010%
8	2.945	495	499	503	rBV2	320	378	0.05%	0.007%
9	3.041	516	529	542	rVB3	9514	18058	2.37%	0.313%
10	3.183	561	573	586	rVB	3925	7684	1.01%	0.133%
11	3.311	608	613	616	rBV2	188	199	0.03%	0.003%
12	3.507	669	674	680	rBV2	148	207	0.03%	0.004%
13	3.649	714	718	724	rBV	183	241	0.03%	0.004%
14	3.768	752	755	760	rVB2	207	174	0.02%	0.003%
15	3.806	764	767	770	rVB	307	203	0.03%	0.004%
16	3.832	770	775	780	rBV2	171	219	0.03%	0.004%
17	3.922	801	803	807	rVB2	301	193	0.03%	0.003%
18	3.967	807	817	823	rBV2	267	496	0.06%	0.009%
19	3.999	823	827	832	rBV2	134	177	0.02%	0.003%
20	4.623	1008	1021	1045	rBV	109745	263841	34.56%	4.567%
21	4.909	1106	1110	1114	rBV3	233	284	0.04%	0.005%
22	5.063	1141	1158	1177	rBV	144641	316052	41.39%	5.470%
23	5.195	1193	1199	1201	rVB3	332	299	0.04%	0.005%
24	5.289	1222	1228	1237	rVB2	900	1385	0.18%	0.024%
25	5.353	1243	1248	1250	rBV	338	198	0.03%	0.003%
26	5.375	1250	1255	1256	rBV2	316	263	0.03%	0.005%
27	5.723	1342	1363	1388	rBV2	278309	763520	100.00%	13.215%
28	5.813	1388	1391	1393	rVB2	390	215	0.03%	0.004%
29	5.851	1400	1403	1405	rBV	324	176	0.02%	0.003%
30	5.925	1423	1426	1434	rVB2	380	333	0.04%	0.006%
31	6.038	1458	1461	1466	rBV3	188	173	0.02%	0.003%
32	6.247	1512	1526	1551	rBV	227790	434043	56.85%	7.513%
33	6.420	1577	1580	1583	rBV	296	225	0.03%	0.004%
34	6.443	1583	1587	1596	rVV	347	383	0.05%	0.007%
35	6.533	1607	1615	1622	rVV3	2212	3514	0.46%	0.061%
36	6.690	1649	1664	1683	rBV	190518	367758	48.17%	6.365%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049837.D
 Acq On : 21 Jul 2022 18:34
 Operator : SY/MD
 Sample : N3792-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.768	1686	1688	1692	rVB3	487	309	0.04%	0.005%
38	6.809	1697	1701	1706	rVB3	612	530	0.07%	0.009%
39	6.838	1706	1710	1713	rBV2	310	218	0.03%	0.004%
40	6.867	1713	1719	1722	rBV2	310	348	0.05%	0.006%
41	7.083	1783	1786	1789	rBV2	232	196	0.03%	0.003%
42	7.147	1801	1806	1810	rBV2	294	333	0.04%	0.006%
43	7.186	1810	1818	1831	rVV4	1590	2740	0.36%	0.047%
44	7.565	1924	1936	1951	rBV	91883	158915	20.81%	2.751%
45	7.690	1969	1975	1985	rVB4	867	1524	0.20%	0.026%
46	7.796	2006	2008	2014	rVB2	462	284	0.04%	0.005%
47	7.899	2027	2040	2056	rBV	304006	519209	68.00%	8.987%
48	8.179	2116	2127	2144	rVV	64710	108691	14.24%	1.881%
49	8.317	2167	2170	2172	rVB2	302	189	0.02%	0.003%
50	8.636	2256	2269	2302	rBV2	275377	536622	70.28%	9.288%
51	8.864	2337	2340	2346	rVB2	450	459	0.06%	0.008%
52	8.919	2353	2357	2360	rBV	354	296	0.04%	0.005%
53	8.973	2369	2374	2380	rBV2	326	441	0.06%	0.008%
54	9.031	2388	2392	2395	rVB	284	206	0.03%	0.004%
55	9.321	2477	2482	2487	rBV2	254	278	0.04%	0.005%
56	9.417	2499	2512	2532	rBV	317989	522155	68.39%	9.038%
57	9.520	2542	2544	2547	rVB3	663	396	0.05%	0.007%
58	9.575	2556	2561	2565	rVB3	372	301	0.04%	0.005%
59	9.645	2579	2583	2588	rVB2	213	232	0.03%	0.004%
60	10.028	2695	2702	2708	rBV2	209	294	0.04%	0.005%
61	10.102	2720	2725	2728	rVV2	456	458	0.06%	0.008%
62	10.121	2729	2731	2734	rVV2	474	328	0.04%	0.006%
63	10.160	2738	2743	2746	rBV2	237	231	0.03%	0.004%
64	10.523	2853	2856	2859	rBV	298	193	0.03%	0.003%
65	10.758	2917	2929	2945	rVV	272827	431100	56.46%	7.462%
66	10.838	2951	2954	2959	rVB3	350	282	0.04%	0.005%
67	10.947	2982	2988	2991	rBV2	246	264	0.03%	0.005%
68	11.018	3001	3010	3013	rBV	251	376	0.05%	0.007%
69	11.041	3013	3017	3020	rVV2	246	199	0.03%	0.003%
70	11.089	3029	3032	3034	rBV2	328	249	0.03%	0.004%
71	11.330	3102	3107	3111	rBV2	234	256	0.03%	0.004%
72	11.353	3111	3114	3118	rBV2	213	217	0.03%	0.004%
73	11.410	3128	3132	3135	rBV2	205	181	0.02%	0.003%
74	11.465	3146	3149	3154	rBV2	375	359	0.05%	0.006%
75	11.812	3243	3257	3286	rBV	268015	429455	56.25%	7.433%
76	11.976	3306	3308	3313	rVB2	337	249	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
 Data File : VU049837.D
 Acq On : 21 Jul 2022 18:34
 Operator : SY/MD
 Sample : N3792-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	12.009	3313	3318	3321	rBV2	262	259	0.03%	0.004%
78	12.195	3362	3376	3396	rBV	273131	443869	58.13%	7.683%
79	12.288	3400	3405	3409	rVB4	532	503	0.07%	0.009%
80	12.346	3418	3423	3425	rBV2	286	236	0.03%	0.004%
81	12.536	3478	3482	3485	rBV	344	240	0.03%	0.004%
82	12.767	3550	3554	3558	rBV	585	489	0.06%	0.008%
83	12.857	3577	3582	3587	rBV2	265	350	0.05%	0.006%
84	12.963	3613	3615	3620	rBV2	272	180	0.02%	0.003%
85	13.089	3650	3654	3661	rBV2	308	352	0.05%	0.006%
86	13.812	3876	3879	3882	rBV2	267	200	0.03%	0.003%
87	13.844	3886	3889	3890	rBV	388	196	0.03%	0.003%
88	13.960	3922	3925	3928	rBV2	328	253	0.03%	0.004%
89	14.060	3953	3956	3960	rVB2	418	286	0.04%	0.005%
90	14.102	3960	3969	3982	rBV4	1457	3009	0.39%	0.052%
91	14.153	3982	3985	3987	rBV3	409	266	0.03%	0.005%
92	14.336	4036	4042	4048	rVB4	943	1197	0.16%	0.021%
93	14.439	4071	4074	4078	rBV3	309	260	0.03%	0.005%
94	14.561	4108	4112	4114	rBV	324	264	0.03%	0.005%
95	14.639	4134	4136	4140	rVB	343	222	0.03%	0.004%
96	14.687	4147	4151	4155	rBV2	347	343	0.04%	0.006%
97	14.806	4182	4188	4190	rBV	430	520	0.07%	0.009%
98	14.931	4224	4227	4228	rBV	280	190	0.02%	0.003%
99	15.944	4539	4542	4544	rBV2	462	269	0.04%	0.005%
100	16.143	4601	4604	4605	rBV	572	303	0.04%	0.005%




Sum of corrected areas: 5777505

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049837.D
Acq On : 21 Jul 2022 18:34
Operator : SY/MD
Sample : N3792-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

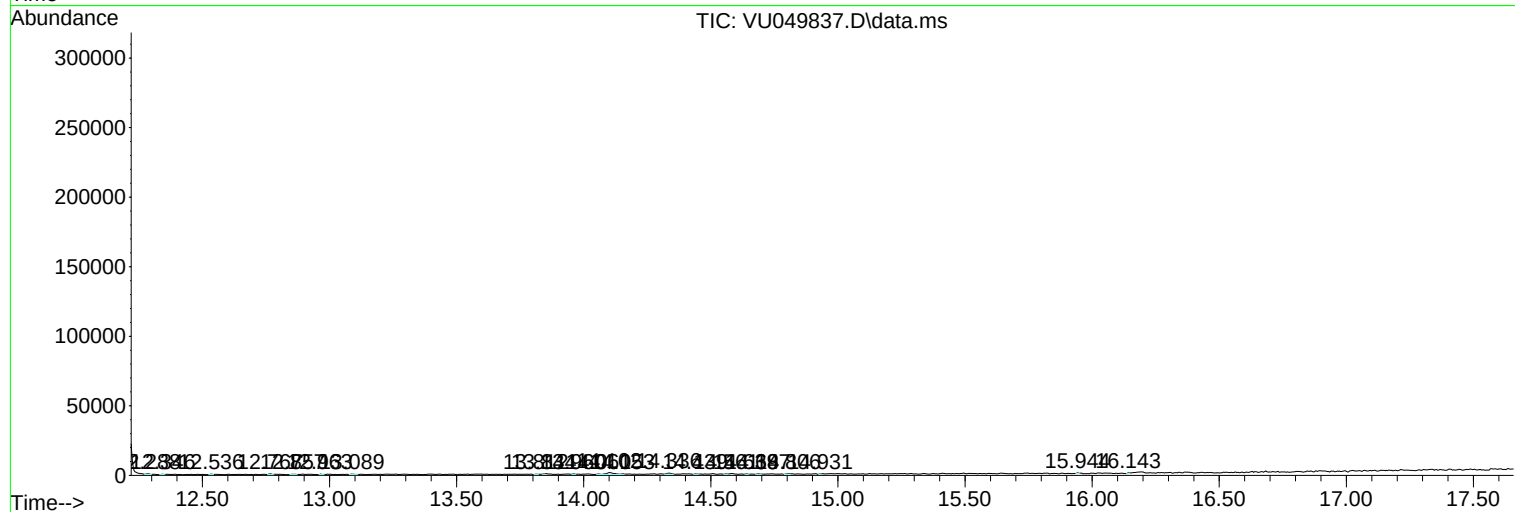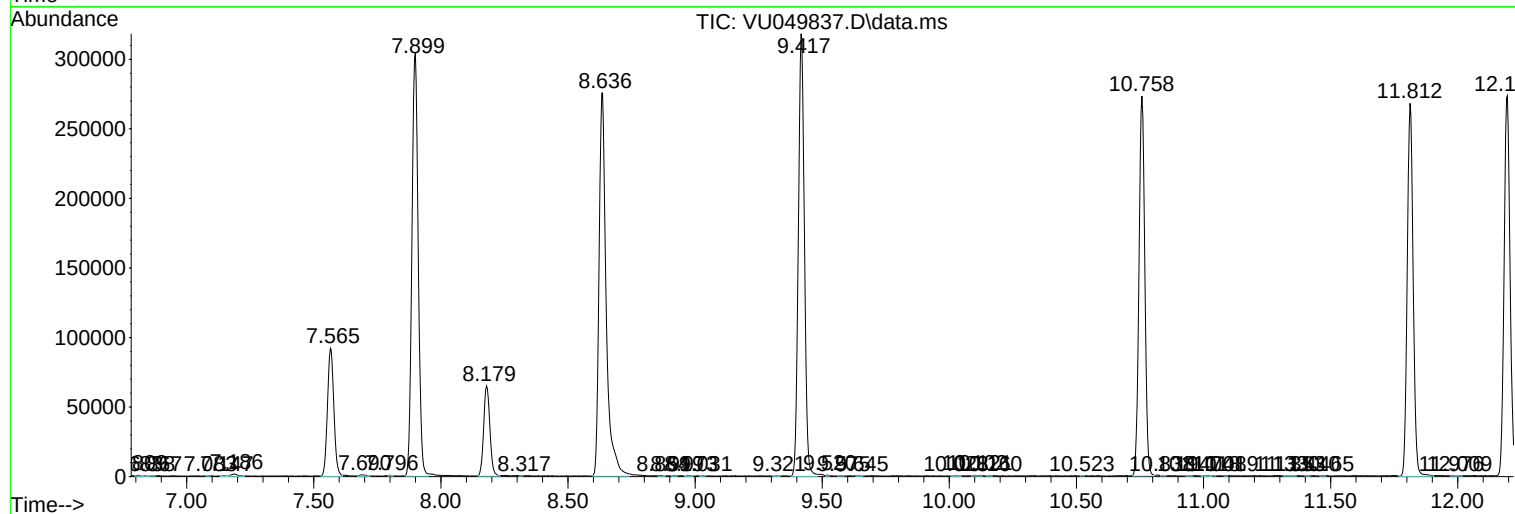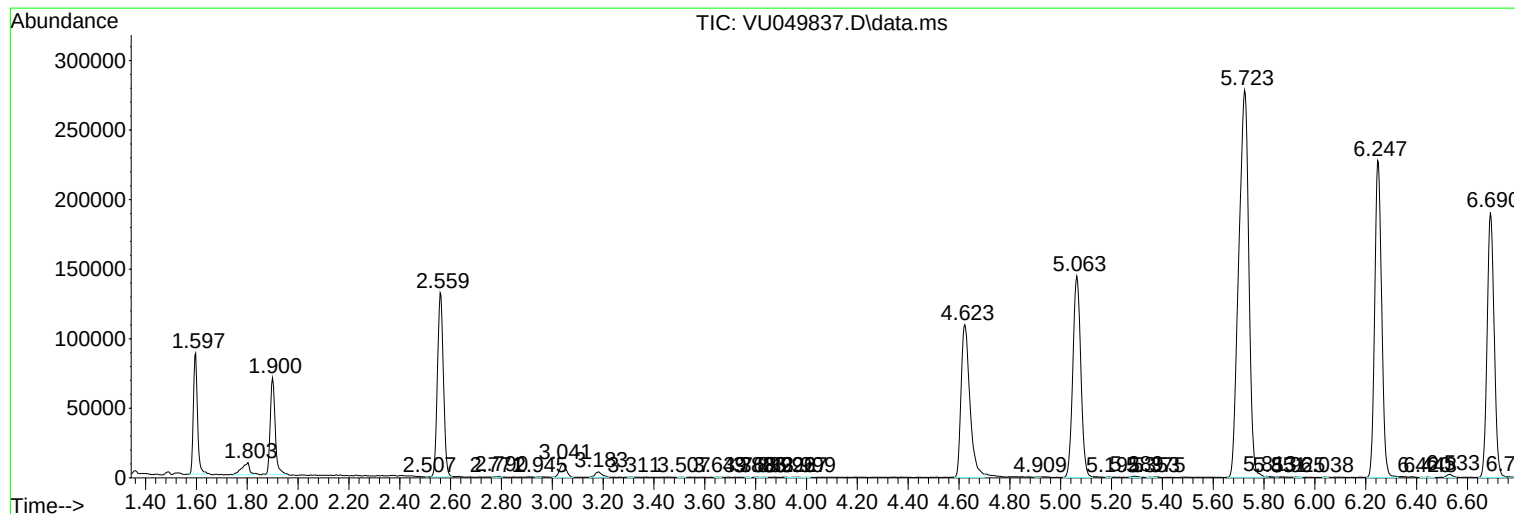

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049837.D
Acq On : 21 Jul 2022 18:34
Operator : SY/MD
Sample : N3792-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049837.D
Acq On : 21 Jul 2022 18:34
Operator : SY/MD
Sample : N3792-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------