


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072122\
Data File : VU049817.D
Acq On : 21 Jul 2022 08:58
Operator : SY/MD
Sample : BFB109
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB109

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Title : VOC Analysis
Last Update : Fri Jul 22 03:08:56 2022

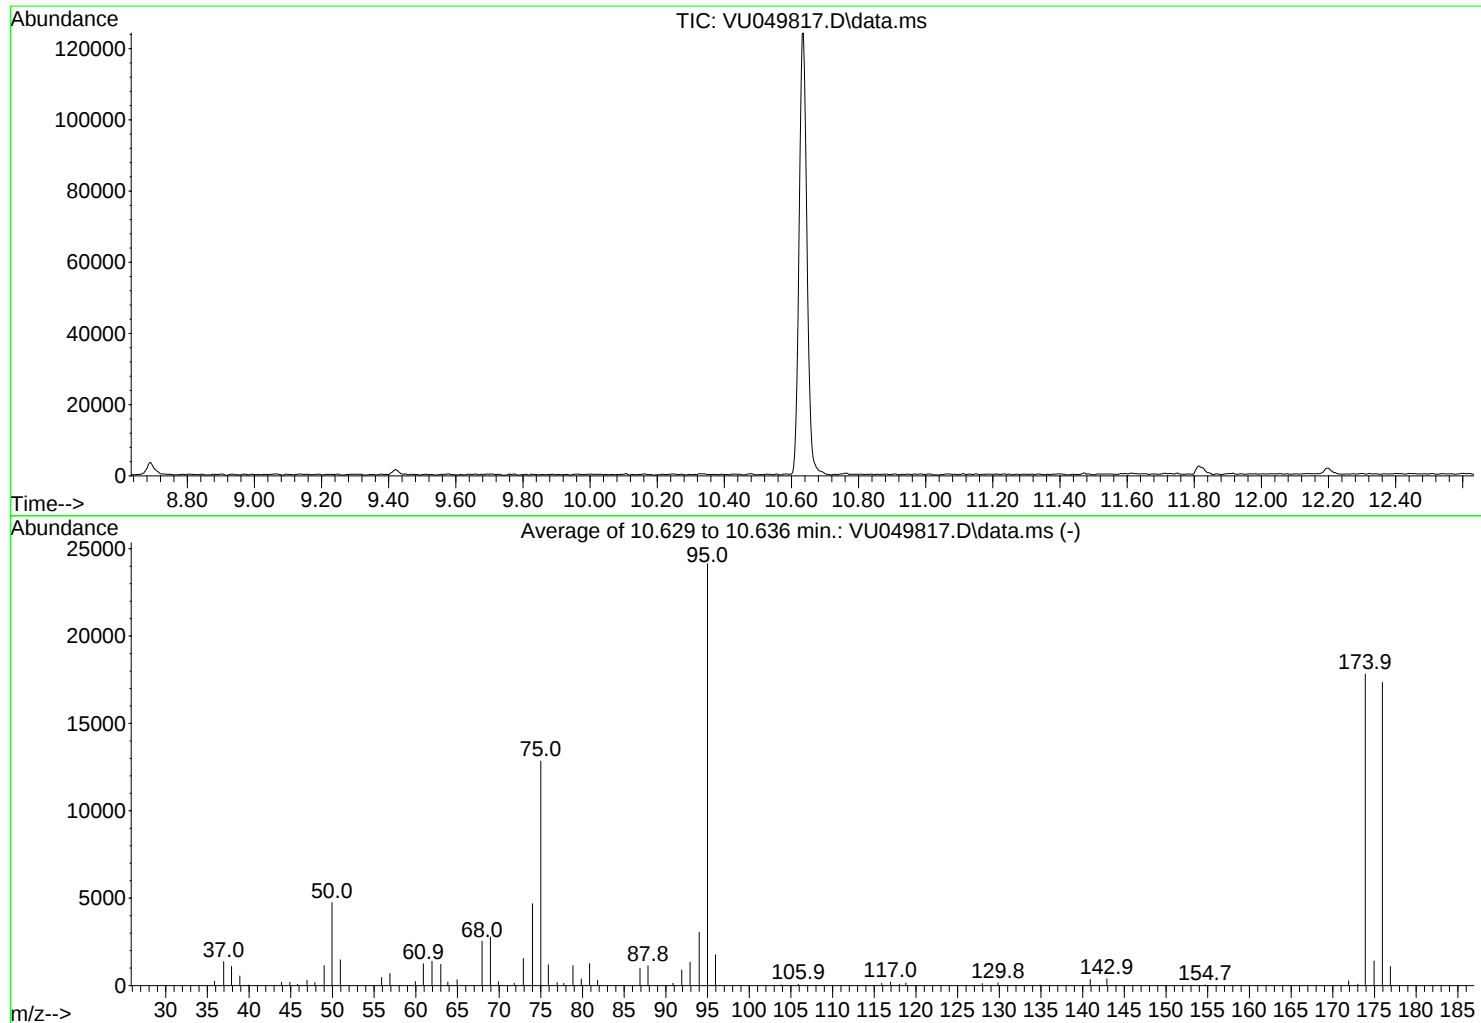

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	4745	PASS
75	95	30	80	53.2	12845	PASS
95	95	100	100	100.0	24139	PASS
96	95	5	9	7.3	1767	PASS
173	174	0.00	2	0.5	81	PASS
174	95	50	120	73.8	17824	PASS
175	174	5	9	7.9	1410	PASS
176	174	95	101	97.3	17346	PASS
177	176	5	9	6.2	1082	PASS

m/z	Abundance
39.90	174.0
43.90	315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB109

m/z	Abundance
35.00	216.0
37.00	1235.0
37.90	990.0
38.90	443.0
40.00	163.0
43.90	573.0
45.00	207.0
45.80	122.0
47.00	322.0
47.90	178.0
49.00	1004.0
49.90	4393.0
51.00	1433.0
55.90	435.0
56.90	612.0
60.00	161.0
60.90	1224.0
61.90	1235.0
63.00	1147.0
63.80	164.0
64.90	291.0
68.00	2364.0
68.90	2690.0
69.90	150.0
71.80	123.0
72.90	1525.0
74.00	4272.0
75.00	12071.0
75.90	1167.0
77.00	191.0
77.80	139.0
78.90	1186.0
79.90	325.0
80.90	1192.0
81.90	245.0
86.90	973.0
87.90	1112.0
90.90	139.0
91.90	841.0
92.90	1278.0
94.00	2892.0
95.00	22800.0
96.00	1646.0
105.90	112.0
115.90	118.0
117.00	188.0
118.80	147.0
127.90	100.0
129.90	131.0
140.90	330.0
142.90	359.0
171.90	198.0
173.00	243.0
173.90	16408.0
174.90	1392.0
176.00	15847.0
176.90	1043.0

Instrument :
MSVOA_U
ClientSampleId :
BFB109

m/z	Abundance
35.80	257.0
37.00	1396.0
37.90	1131.0
38.90	548.0
39.90	209.0
43.90	517.0
44.90	184.0
45.80	100.0
47.00	297.0
47.90	183.0
49.00	1219.0
50.00	4929.0
51.00	1510.0
55.90	508.0
56.90	717.0
60.00	252.0
60.90	1275.0
61.90	1402.0
63.00	1238.0
63.80	221.0
65.00	345.0
67.90	2615.0
68.90	2916.0
69.90	216.0
71.80	146.0
72.90	1644.0
74.00	4882.0
75.00	13025.0
75.90	1232.0
76.90	172.0
77.80	127.0
78.80	1183.0
79.80	369.0
80.90	1299.0
81.80	298.0
86.90	1040.0
87.90	1202.0
90.80	130.0
91.90	939.0
92.90	1415.0
94.00	3138.0
95.00	24872.0
96.00	1809.0
105.90	118.0
115.90	139.0
117.00	207.0
118.00	107.0
118.80	158.0
128.00	123.0
129.90	178.0
140.90	349.0
142.90	397.0
171.90	271.0
173.90	18392.0
174.90	1457.0
175.90	17984.0
176.90	1093.0

Instrument :
MSVOA_U
ClientSampleId :
BFB109

m/z	Abundance
35.90	243.0
36.90	1481.0
37.90	1151.0
38.90	642.0
39.90	245.0
43.90	443.0
44.80	174.0
46.80	266.0
47.90	162.0
49.00	1209.0
49.90	4913.0
50.90	1479.0
55.90	438.0
56.90	759.0
59.90	298.0
60.90	1257.0
62.00	1521.0
63.00	1263.0
63.90	223.0
65.00	358.0
67.90	2619.0
69.00	2744.0
69.90	270.0
71.80	125.0
72.90	1469.0
74.00	4886.0
75.00	13439.0
75.90	1174.0
76.90	156.0
77.70	100.0
78.80	1050.0
79.80	437.0
80.80	1273.0
81.70	344.0
86.90	979.0
87.80	1083.0
90.80	132.0
91.90	879.0
92.90	1313.0
94.00	3105.0
95.00	24744.0
95.90	1847.0
103.80	117.0
115.90	138.0
116.90	184.0
118.00	118.0
118.80	147.0
128.00	118.0
129.80	167.0
134.90	118.0
140.90	353.0
142.90	408.0
154.70	101.0
171.90	334.0
173.90	18672.0
175.00	1381.0
175.90	18208.0
176.90	1110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB109