


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072123\
Data File : VU054835.D
Acq On : 21 Jul 2023 08:33
Operator : MD/SY
Sample : BFB032
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB032

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM072023.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jul 21 01:10:23 2023

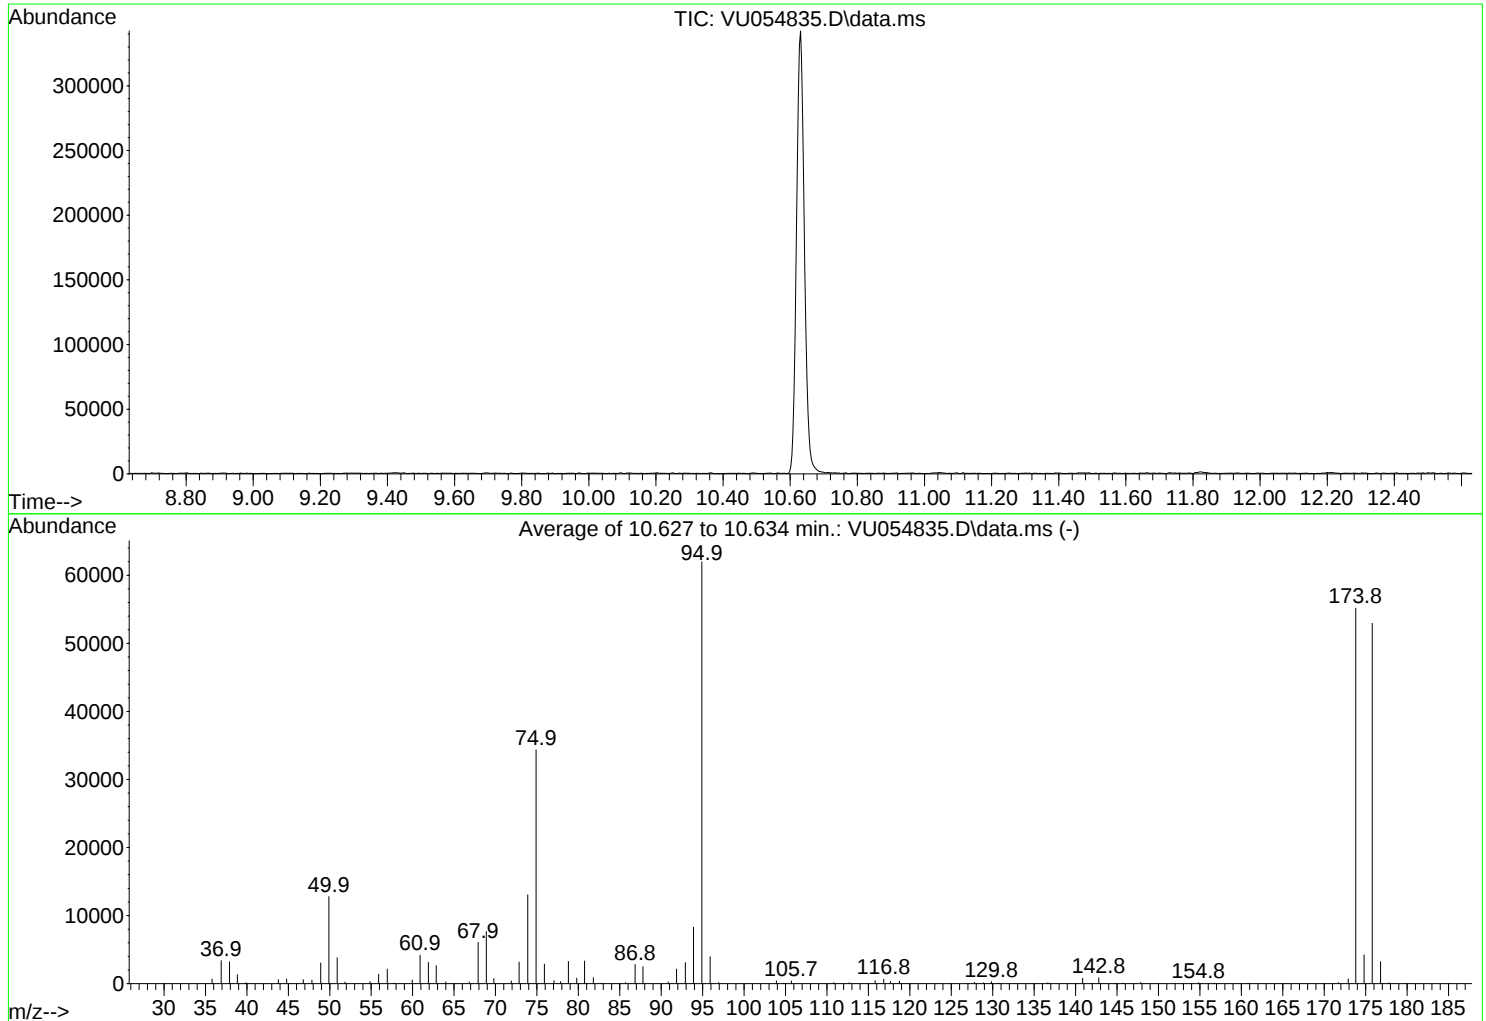

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	12787	PASS
75	95	30	80	55.4	34349	PASS
95	95	100	100	100.0	61979	PASS
96	95	5	9	6.4	3950	PASS
173	174	0.00	2	1.3	701	PASS
174	95	50	120	89.0	55192	PASS
175	174	5	9	7.7	4235	PASS
176	174	95	101	95.9	52939	PASS
177	176	5	9	6.1	3231	PASS

m/z	Abundance
42.60	101.0
43.90	276.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.80	626.0
36.90	3314.0
37.90	3383.0
38.90	1231.0
39.90	156.0
43.80	886.0
44.80	664.0
46.80	657.0
47.80	506.0
48.90	3180.0
49.90	13073.0
50.90	3959.0
51.90	220.0
54.80	310.0
55.80	1405.0
57.00	2181.0
60.00	533.0
60.90	4215.0
61.90	3412.0
62.90	2796.0
64.00	219.0
66.80	228.0
67.90	6213.0
68.90	7540.0
69.80	721.0
71.90	428.0
72.90	3240.0
73.90	13123.0
74.90	34472.0
75.90	2956.0
77.00	510.0
77.90	261.0
78.80	3356.0
79.80	761.0
80.80	3410.0
81.80	877.0
82.80	108.0
85.70	151.0
86.80	2921.0
87.80	2443.0
90.80	317.0
91.80	2188.0
92.90	2954.0
93.90	8157.0
94.90	62712.0
95.90	3969.0
96.90	186.0
103.90	376.0
105.70	366.0
110.80	140.0
112.60	132.0
115.80	522.0
116.80	605.0
117.60	296.0
118.80	386.0
127.80	219.0
128.90	124.0
129.80	286.0
136.60	135.0
140.80	745.0
142.80	808.0
145.70	150.0
147.90	167.0
154.90	107.0
171.70	232.0
172.90	744.0
173.80	54736.0
174.80	4247.0
175.80	51624.0
176.80	3185.0
177.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.80	671.0
36.90	3521.0
37.90	3226.0
38.80	1324.0
39.90	151.0
42.50	106.0
43.80	881.0
44.80	675.0
46.80	604.0
47.90	557.0
48.90	3200.0
49.90	13120.0
50.90	3907.0
51.90	247.0
54.80	288.0
55.90	1417.0
57.00	2165.0
57.80	104.0
60.00	566.0
60.90	4431.0
61.90	3138.0
62.80	2697.0
64.00	271.0
66.80	266.0
67.90	6110.0
68.90	8013.0
69.80	800.0
71.90	421.0
72.90	3230.0
73.90	13506.0
74.90	35392.0
75.90	3003.0
77.10	460.0
77.80	319.0
78.80	3397.0
79.80	830.0
80.70	3376.0
81.80	900.0
82.80	121.0
85.70	202.0
86.80	2851.0
87.80	2514.0
90.90	254.0
91.90	2185.0
92.90	3238.0
93.90	8584.0
94.90	64248.0
95.90	4080.0
96.90	187.0
103.90	421.0
104.80	105.0
105.70	417.0
110.80	142.0
112.70	139.0
115.80	485.0
116.90	701.0
117.70	293.0
118.80	344.0
127.80	190.0
128.90	139.0
129.90	334.0
130.70	102.0
136.60	138.0
140.90	781.0
142.80	854.0
145.70	146.0
147.90	220.0
154.80	146.0
156.70	118.0
160.80	100.0
171.70	152.0
172.90	750.0
173.80	56928.0
174.80	4361.0
175.80	54624.0
176.80	3297.0
177.80	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.80	721.0
36.90	3354.0
37.90	3015.0
38.80	1418.0
39.90	132.0
42.60	131.0
43.80	816.0
44.80	743.0
46.80	512.0
47.90	493.0
48.90	2702.0
49.90	12169.0
50.90	3534.0
51.80	222.0
54.90	272.0
56.00	1337.0
56.90	2092.0
57.70	155.0
59.90	561.0
60.90	3906.0
61.90	2810.0
62.90	2506.0
64.00	277.0
66.90	245.0
67.90	5870.0
68.90	7465.0
69.80	725.0
71.90	372.0
72.80	3060.0
73.90	12497.0
74.90	33184.0
75.90	2652.0
77.10	384.0
77.90	293.0
78.80	3066.0
79.80	781.0
80.80	3144.0
81.80	804.0
85.70	164.0
86.90	2690.0
87.80	2488.0
90.80	222.0
91.90	2028.0
92.90	3025.0
93.90	8086.0
94.90	58976.0
95.90	3800.0
96.90	154.0
103.90	377.0
104.80	140.0
105.70	428.0
110.80	114.0
112.70	112.0
115.80	362.0
116.90	670.0
117.70	312.0
118.70	315.0
127.90	130.0
128.90	121.0
129.90	322.0
130.70	122.0
136.70	133.0
140.90	807.0
141.90	112.0
142.80	863.0
144.80	105.0
147.80	204.0
151.60	108.0
154.80	165.0
156.80	105.0
160.80	110.0
171.80	112.0
172.90	609.0
173.80	53912.0
174.80	4096.0
175.80	52568.0
176.80	3211.0
177.80	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032