


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072219\
Data File : VU033359.D
Acq On : 22 Jul 2019 17:15
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072219DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Jul 23 03:43:51 2019

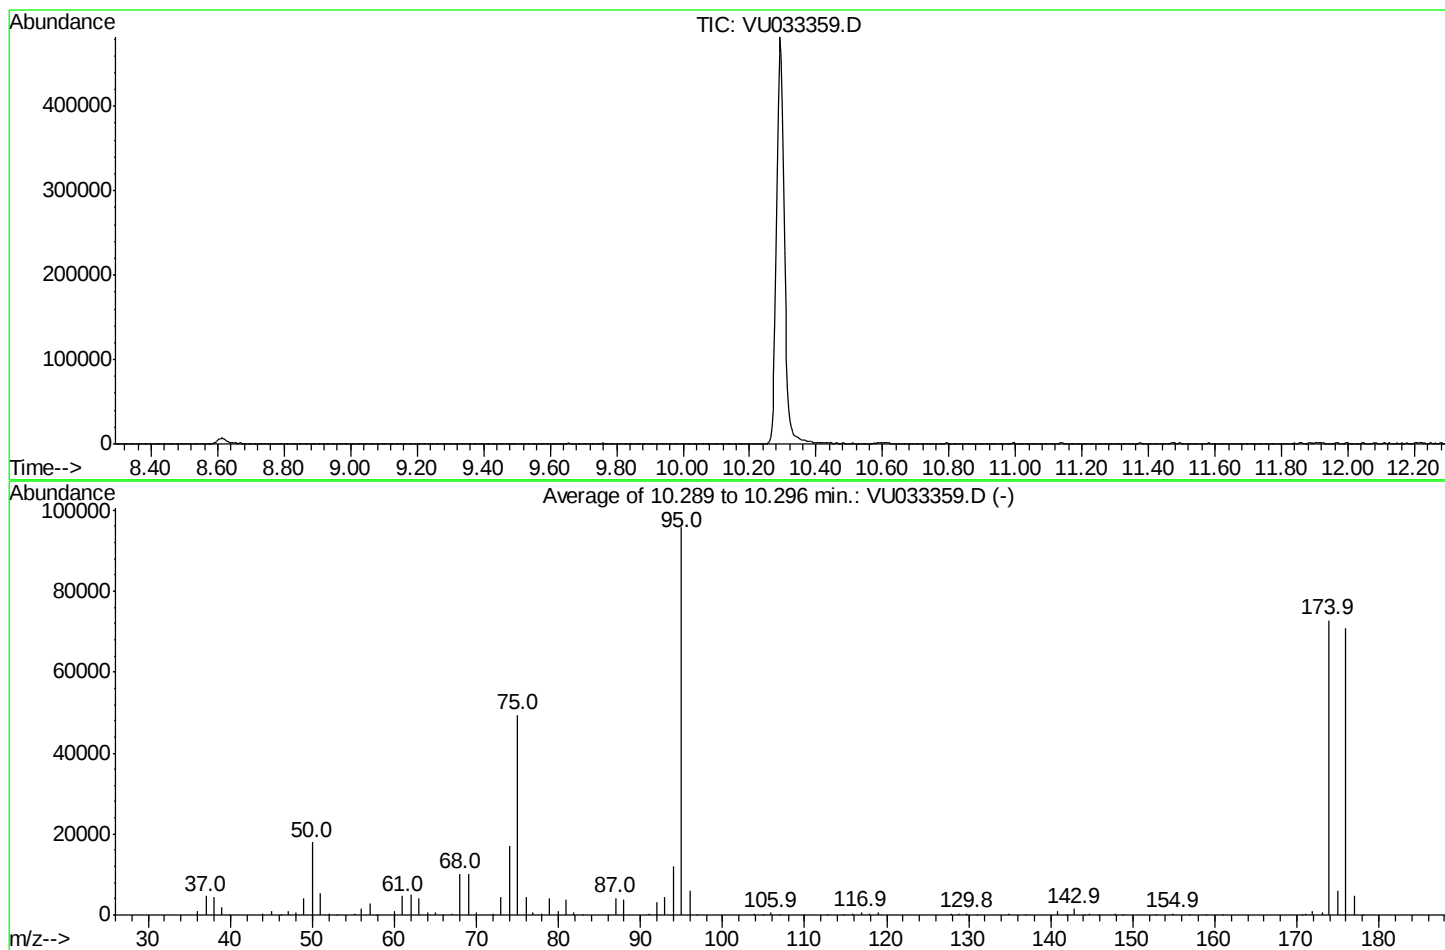

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	17936	PASS
75	95	30	60	51.6	49408	PASS
95	95	100	100	100.0	95781	PASS
96	95	5	9	6.3	5994	PASS
173	174	0.00	2	0.7	499	PASS
174	95	50	100	76.0	72805	PASS
175	174	5	9	8.2	5954	PASS
176	174	95	101	97.2	70754	PASS
177	176	5	9	6.5	4632	PASS