

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072220\
Data File : VU039625.D
Acq On : 22 Jul 2020 12:56
Operator : SY/MD
Sample : L3347-11DL 5X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAY03DL

Manual Integrations
APPROVED

MMDadoda
7/23/2020 12:09:39 PM

Quant Time: Jul 23 01:30:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 23 01:28:13 2020
Response via : Initial Calibration

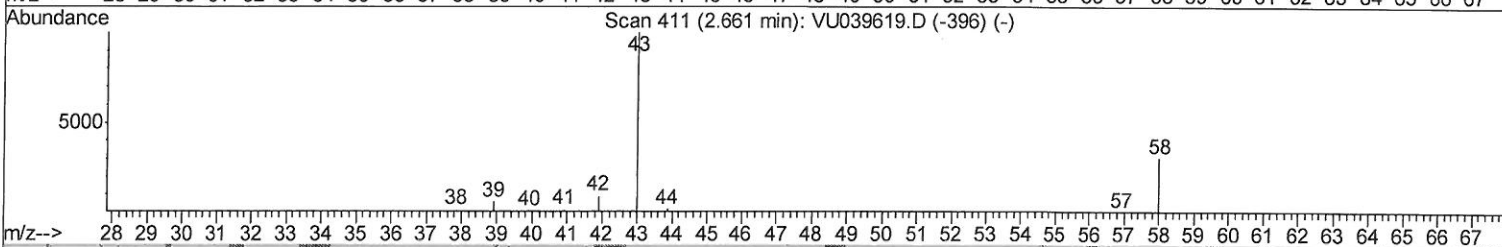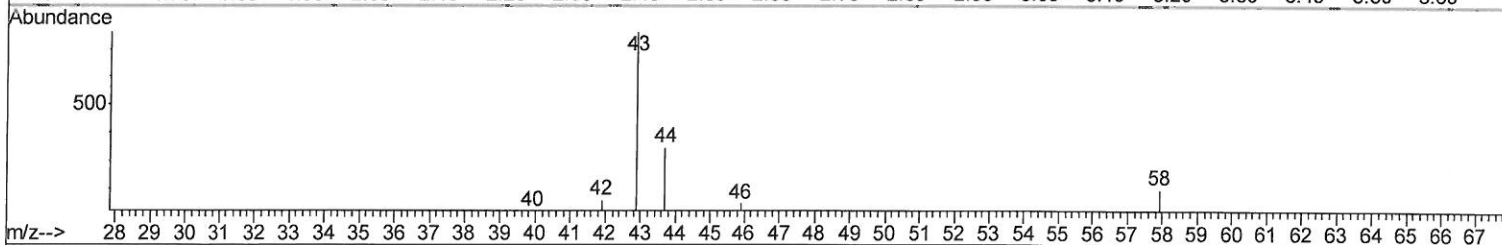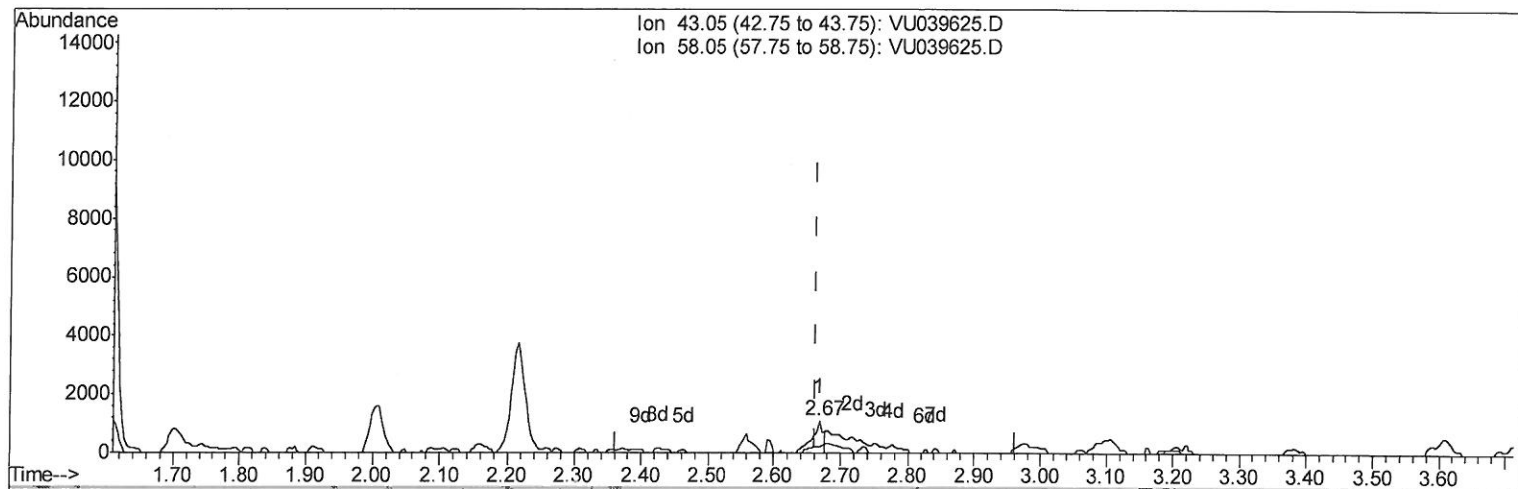

TIC: VU039625.D

(13) Acetone (T)

2.668min (+0.007) 0.90ug/L

response 1212

Ion	Exp%	Act%
43.05	100	100
58.05	29.50	78.47#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072220\
 Data File : VU039625.D
 Acq On : 22 Jul 2020 12:56
 Operator : SY/MD
 Sample : L3347-11DL 5X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAY03DL

Manual Integrations
 APPROVED

MMDadoda
 7/23/2020 12:09:39 PM

Quant Time: Jul 23 01:30:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 23 01:28:13 2020
 Response via : Initial Calibration

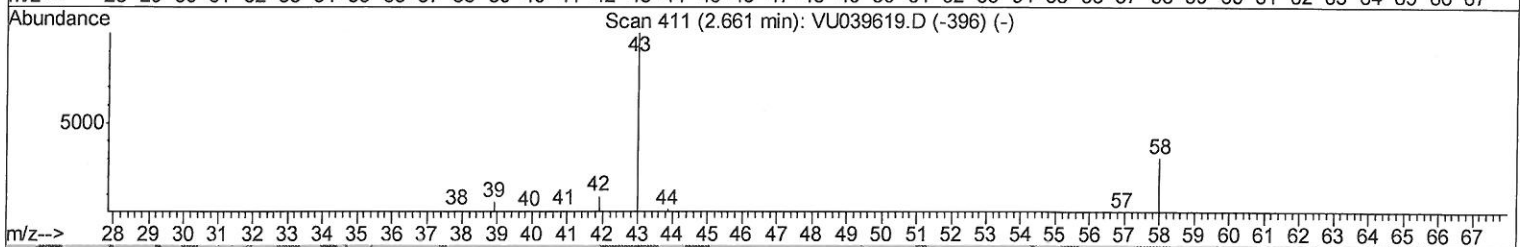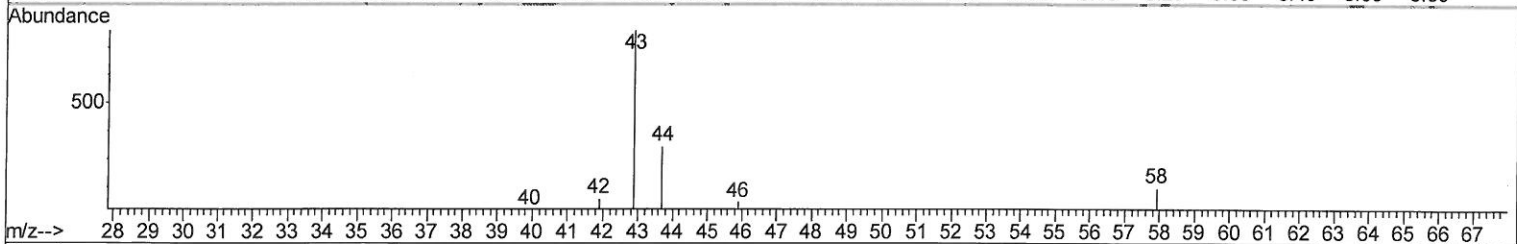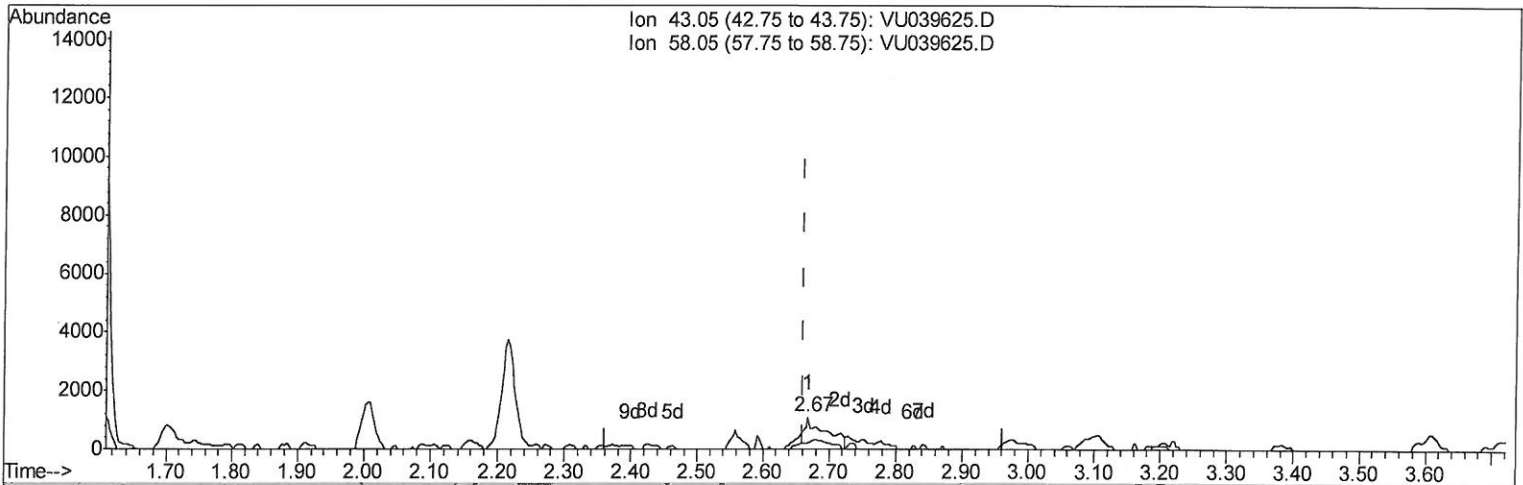

(13) Acetone (T)

2.668min (+0.007) 2.12ug/L m

response 2866

Ion	Exp%	Act%
43.05	100	100
58.05	29.50	33.18
0.00	0.00	0.00
0.00	0.00	0.00

507/28/20 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072220\
 Data File : VU039625.D
 Acq On : 22 Jul 2020 12:56
 Operator : SY/MD
 Sample : L3347-11DL 5X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 GAY03DL

Manual Integrations
 APPROVED

MMDadoda
 7/23/2020 12:09:39 PM

Quant Time: Jul 23 02:18:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 23 01:28:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	115960	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	109080	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	50819	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.61	65	26791	4.98	ug/L	0.00
Spiked Amount 5.000	Range	40 - 130	Recovery	=	99.60%	
7) Chloroethane-d5	1.92	69	24687	4.20	ug/L	0.00
Spiked Amount 5.000	Range	65 - 130	Recovery	=	84.00%	
11) 1,1-Dichloroethene-d2	2.58	63	46242	3.82	ug/L	0.00
Spiked Amount 5.000	Range	60 - 125	Recovery	=	76.40%	
20) 2-Butanone-d5	4.66	46	108440	44.67	ug/L	0.00
Spiked Amount 50.000	Range	40 - 130	Recovery	=	89.34%	
24) Chloroform-d	5.08	84	54890	4.02	ug/L	0.00
Spiked Amount 5.000	Range	70 - 125	Recovery	=	80.40%	
26) 1,2-Dichloroethane-d4	5.72	65	37840	4.20	ug/L	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	84.00%	
32) Benzene-d6	5.75	84	113434	4.33	ug/L	0.00
Spiked Amount 5.000	Range	70 - 125	Recovery	=	86.60%	
36) 1,2-Dichloropropane-d6	6.70	67	37115	4.30	ug/L	0.00
Spiked Amount 5.000	Range	60 - 140	Recovery	=	86.00%	
41) Toluene-d8	7.91	98	99930	4.02	ug/L	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	80.40%	
43) trans-1,3-Dichloropropene-	8.19	79	13974	3.72	ug/L	0.00
Spiked Amount 5.000	Range	55 - 130	Recovery	=	74.40%	
46) 2-Hexanone-d5	8.64	63	74925	40.83	ug/L	0.00
Spiked Amount 50.000	Range	45 - 130	Recovery	=	81.66%	
57) 1,1,2,2-Tetrachloroethane-	10.76	84	31607	3.94	ug/L	0.00
Spiked Amount 5.000	Range	65 - 120	Recovery	=	78.80%	
64) 1,2-Dichlorobenzene-d4	12.19	152	38748	4.24	ug/L	0.00
Spiked Amount 5.000	Range	80 - 120	Recovery	=	84.80%	
Target Compounds						
13) Acetone	2.67	43	2866m	2.121	ug/L	Ovalue
25) Chloroform	5.11	83	5964	0.419	ug/L	96
42) Toluene	7.97	91	2775	0.097	ug/L	100
47) Tetrachloroethene	8.56	164	27310	5.531	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072220\
Data File : VU039625.D
Acq On : 22 Jul 2020 12:56
Operator : SY/MD
Sample : L3347-11DL 5X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAY03DL

Manual Integrations
APPROVED

MMDadoda
7/23/2020 12:09:39 PM

Quant Time: Jul 23 02:18:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 23 01:28:13 2020
Response via : Initial Calibration

