


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072220\
 Data File : VU039618.D
 Acq On : 22 Jul 2020 08:53
 Operator : SY/MD
 Sample : BFB07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB07

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 23 01:28:13 2020

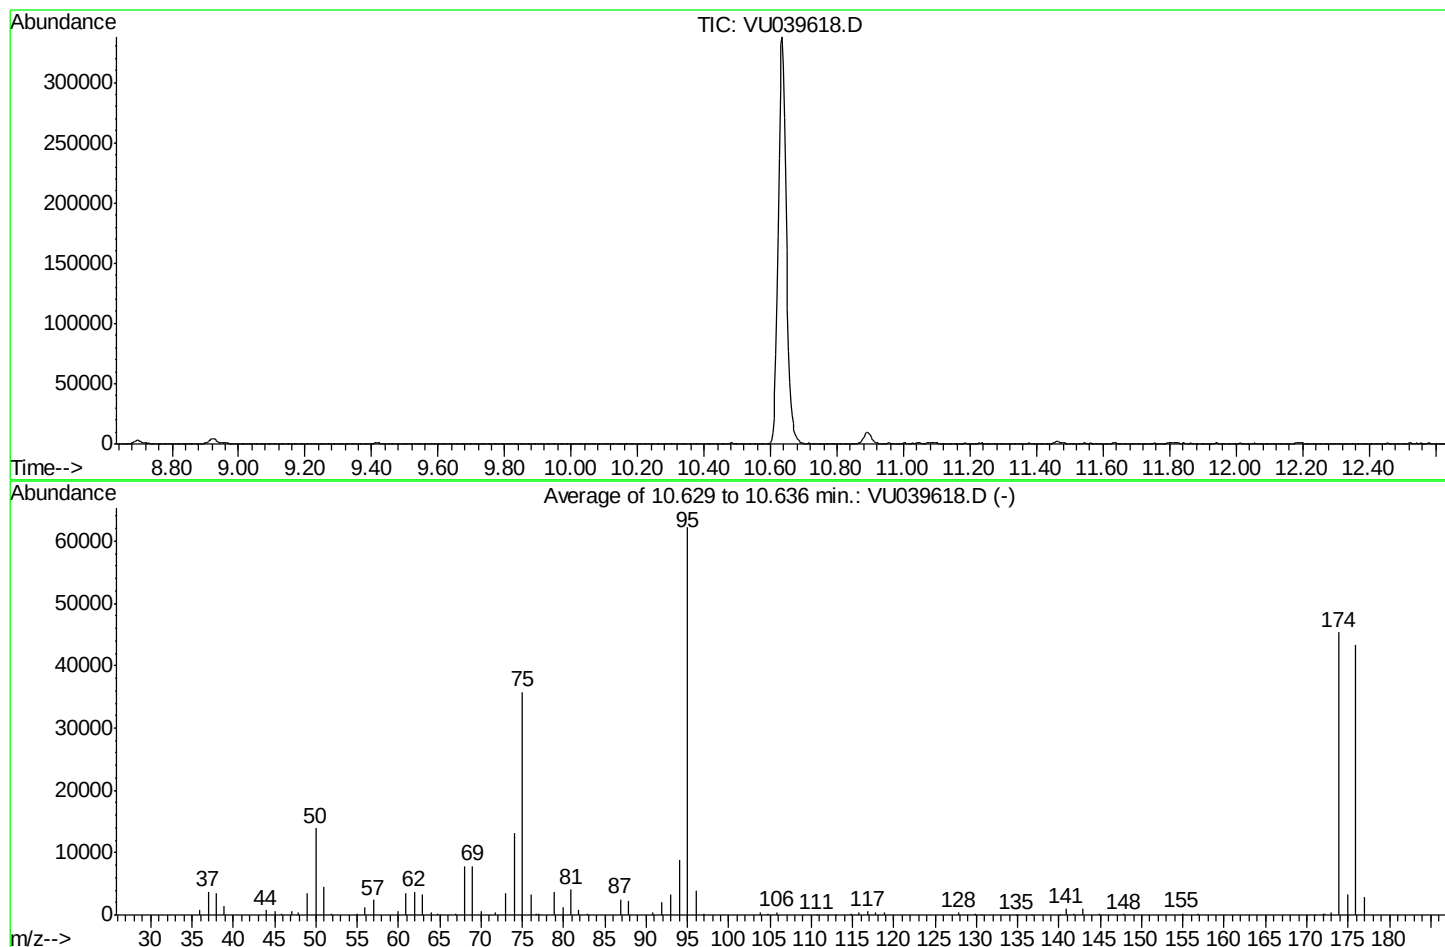

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	13937	PASS
75	95	30	80	57.5	35768	PASS
95	95	100	100	100.0	62210	PASS
96	95	5	9	6.4	4005	PASS
173	174	0.00	2	1.1	501	PASS
174	95	50	120	72.9	45368	PASS
175	174	5	9	7.3	3326	PASS
176	174	95	101	95.8	43450	PASS
177	176	5	9	6.5	2843	PASS

m/z	Abundance
35.90	837.0
37.00	3752.0
38.00	3582.0
38.90	1395.0
39.90	150.0
44.00	1123.0
45.00	511.0
45.90	146.0
47.10	689.0
47.80	466.0
49.00	3186.0
50.00	13027.0
51.00	4313.0
52.00	195.0
55.00	155.0
55.90	1213.0
57.00	2297.0
59.90	550.0
60.90	3253.0
61.90	3594.0
62.90	3012.0
63.90	275.0
64.80	207.0
67.00	179.0
68.00	7201.0
69.00	7348.0
69.90	596.0
71.80	373.0
73.00	3332.0
74.00	12083.0
75.00	32632.0
76.00	2956.0
77.00	297.0
78.80	3402.0
79.90	1065.0
80.90	3931.0
81.80	708.0
82.80	110.0
86.90	2270.0
87.90	2252.0
90.90	401.0
91.90	1751.0
93.00	3162.0
94.00	8259.0
95.00	58392.0
96.00	3627.0
97.00	133.0
103.80	341.0
104.80	107.0
105.80	371.0
114.80	200.0
115.80	362.0
116.90	440.0
117.80	327.0
118.90	375.0
127.90	283.0
129.80	250.0
140.90	880.0
141.80	101.0
142.90	822.0
144.90	163.0
148.00	112.0
154.90	148.0
156.90	141.0
171.90	357.0
173.00	410.0
173.90	40344.0
175.00	2881.0
175.90	38792.0
176.90	2532.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
35.90	890.0
37.00	3880.0
38.00	3615.0
38.90	1560.0
39.90	120.0
44.00	1119.0
45.00	615.0
45.90	124.0
47.10	691.0
47.90	433.0
49.00	3577.0
50.00	14341.0
51.00	4681.0
51.90	249.0
55.00	173.0
55.90	1354.0
57.00	2532.0
59.90	705.0
60.90	3540.0
61.90	3920.0
62.90	3414.0
63.90	369.0
64.80	206.0
67.00	163.0
68.00	8013.0
69.00	8124.0
70.00	657.0
71.80	375.0
73.00	3646.0
74.00	13501.0
75.00	36736.0
76.00	3354.0
76.90	319.0
78.80	3922.0
79.90	1214.0
80.90	4164.0
81.80	892.0
82.90	160.0
86.90	2592.0
87.90	2324.0
90.80	423.0
91.90	2136.0
93.00	3462.0
94.00	9054.0
95.00	64200.0
96.00	4163.0
97.00	113.0
103.80	389.0
104.80	138.0
105.80	479.0
110.70	112.0
112.90	123.0
114.80	194.0
115.80	327.0
116.90	576.0
117.80	370.0
118.80	411.0
127.90	341.0
129.80	318.0
134.90	134.0
136.70	124.0
140.10	102.0
140.90	1073.0
141.80	133.0
142.90	966.0
145.00	192.0
147.90	111.0
154.90	230.0
156.90	168.0
171.00	120.0
172.00	334.0
173.00	503.0
173.90	46816.0
175.00	3426.0
175.90	44888.0
176.90	2874.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
35.90	809.0
37.00	3724.0
37.90	3488.0
38.90	1686.0
39.90	114.0
44.00	968.0
45.00	700.0
45.90	127.0
47.00	599.0
47.90	390.0
49.00	3445.0
50.00	14445.0
51.00	4671.0
51.90	280.0
55.00	189.0
56.00	1427.0
57.00	2459.0
59.90	785.0
60.90	3592.0
61.90	3762.0
63.00	3425.0
63.90	355.0
65.00	201.0
66.90	162.0
67.90	8067.0
69.00	8072.0
70.00	722.0
71.80	318.0
73.00	3612.0
74.00	13925.0
75.00	37936.0
76.00	3459.0
76.70	359.0
78.80	4005.0
79.90	1220.0
80.90	4057.0
81.80	990.0
83.00	177.0
86.90	2568.0
87.90	2174.0
90.80	422.0
91.90	2311.0
93.00	3334.0
94.00	9048.0
95.00	64040.0
96.00	4225.0
97.00	110.0
103.80	391.0
104.80	140.0
105.90	502.0
110.70	100.0
112.90	133.0
114.80	143.0
115.80	293.0
116.90	671.0
117.80	374.0
118.80	387.0
127.90	334.0
129.80	368.0
130.70	116.0
134.80	168.0
136.80	137.0
140.10	101.0
140.90	1092.0
141.90	153.0
142.90	1051.0
145.00	158.0
147.80	133.0
154.90	253.0
156.90	174.0
170.90	107.0
172.20	374.0
173.00	591.0
173.90	48944.0
174.90	3673.0
175.90	46672.0
176.90	3123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

Scan 2876 (10.587 min): VU039618.D
BFB07

m/z	Abundance
39.90	155.0
43.90	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07