

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072221\
 Data File : VU044385.D
 Acq On : 22 Jul 2021 11:03
 Operator : SY/MD
 Sample : VU0722WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0722WBL01

Quant Time: Jul 23 03:28:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 16 14:36:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.121	96	46556	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.639	95	17355	0.924	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	16803	0.917	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	
Target Compounds						
15) Methylene Chloride	3.054	84	6532	0.387	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072221\
Data File : VU044385.D
Acq On : 22 Jul 2021 11:03
Operator : SY/MD
Sample : VU07222WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0722WBL01

Quant Time: Jul 23 03:28:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 16 14:36:39 2021
Response via : Initial Calibration

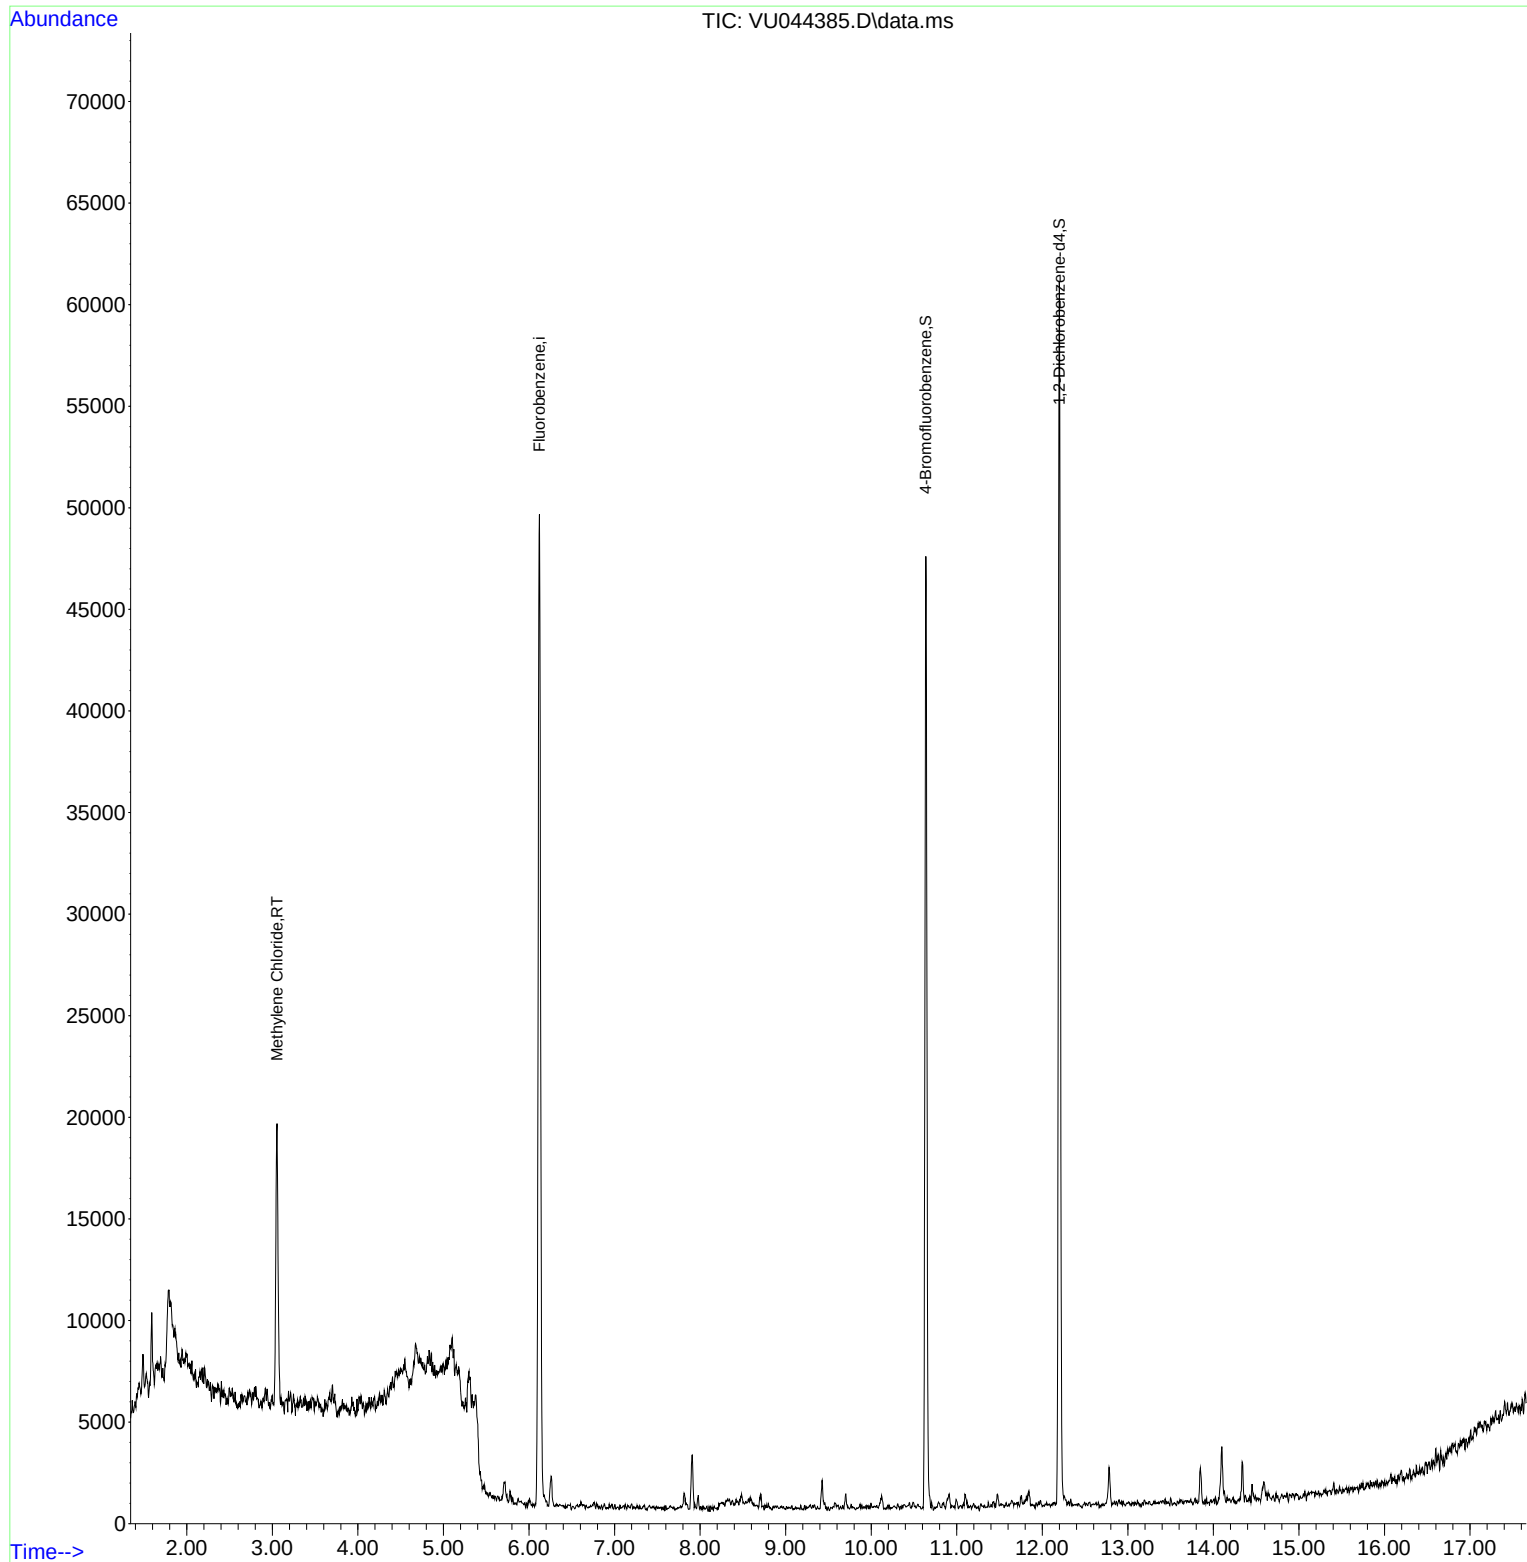




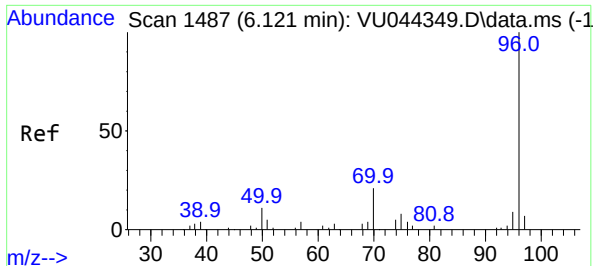


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.121 min Scan# 1487
Delta R.T. 0.000 min
Lab File: VU044385.D
Acq: 22 Jul 2021 11:03

Instrument :
MSVOA_U
ClientSampleId :
VU0722WBL01

Tgt Ion: 96 Resp: 46556




Ion	Ratio	Lower	Upper
96	100		
70	21.0	16.2	24.2
95	8.6	7.3	10.9
97	6.6	0.0	0.0#

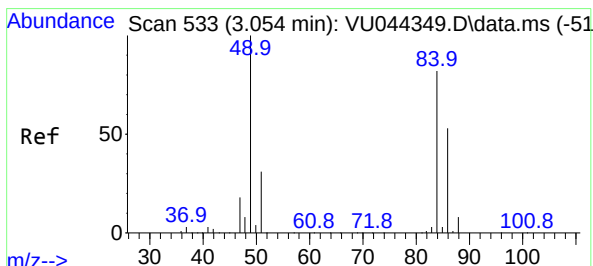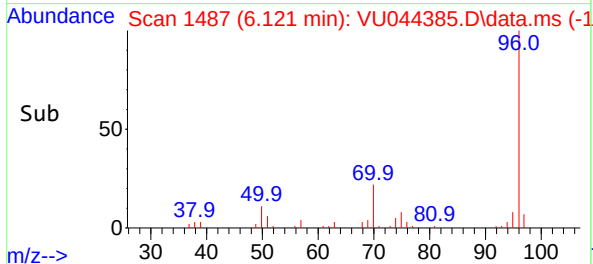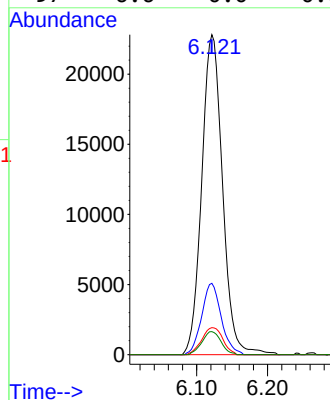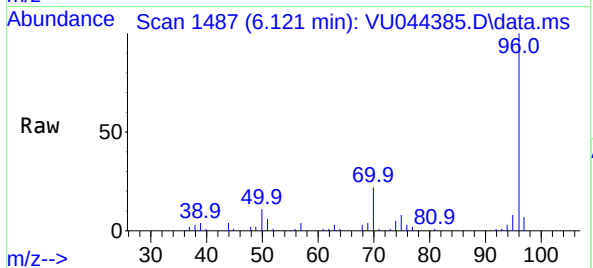


#15
Methylene Chloride
Concen: 0.387 ug/l
RT: 3.054 min Scan# 533
Delta R.T. 0.000 min
Lab File: VU044385.D
Acq: 22 Jul 2021 11:03

Tgt Ion: 84 Resp: 6532

Ion	Ratio	Lower	Upper
84	100		
49	124.6	106.3	159.5
51	35.6	0.0	81.8
86	63.2	51.4	77.0


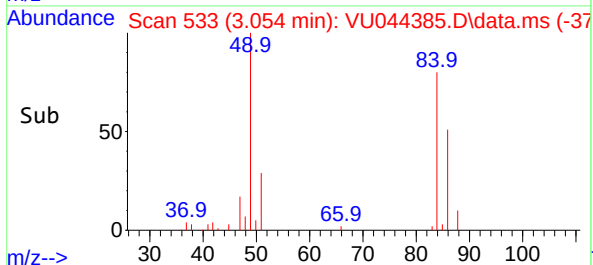
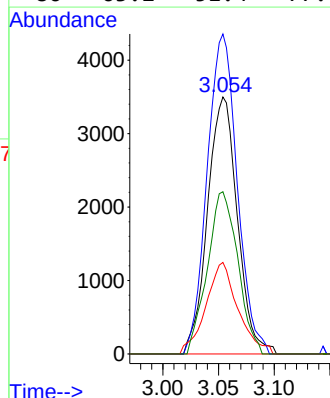
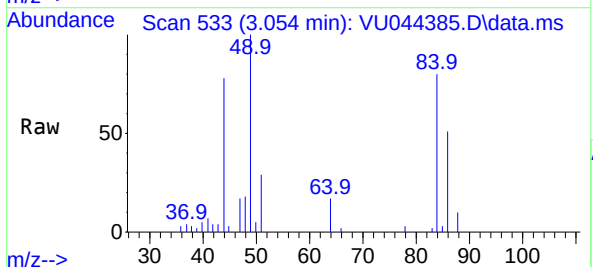


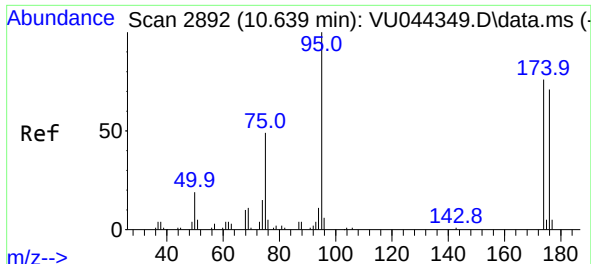

#57
4-Bromofluorobenzene
Concen: 0.924 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.000 min
Lab File: VU044385.D
Acq: 22 Jul 2021 11:03

Instrument :
MSVOA_U
ClientSampleId :
VU0722WBL01

Tgt Ion: 95 Resp: 17355
Ion Ratio Lower Upper
95 100
174 72.7 62.2 93.2
176 68.9 60.3 90.5

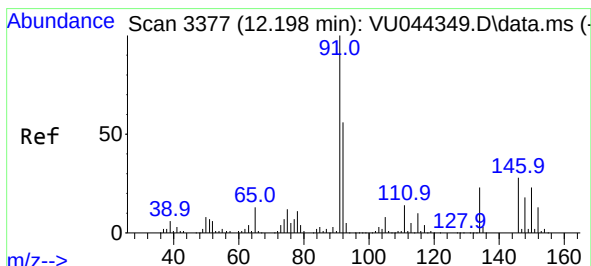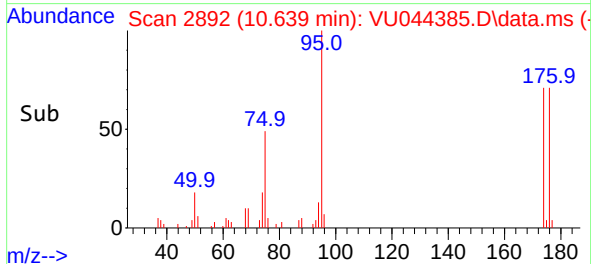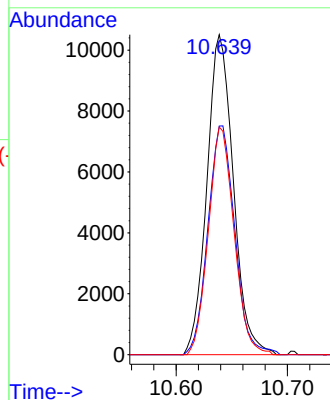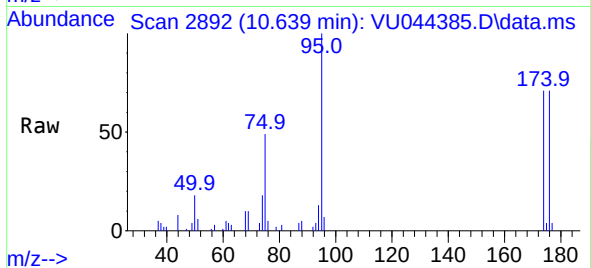

#68
1,2-Dichlorobenzene-d4
Concen: 0.917 ug/l
RT: 12.198 min Scan# 3377
Delta R.T. 0.000 min
Lab File: VU044385.D
Acq: 22 Jul 2021 11:03

Tgt Ion: 152 Resp: 16803
Ion Ratio Lower Upper
152 100
115 62.8 0.0 257.0
150 154.4 0.0 630.2

