


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072221\
Data File : VU044383.D
Acq On : 22 Jul 2021 09:33
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Jul 16 14:36:39 2021

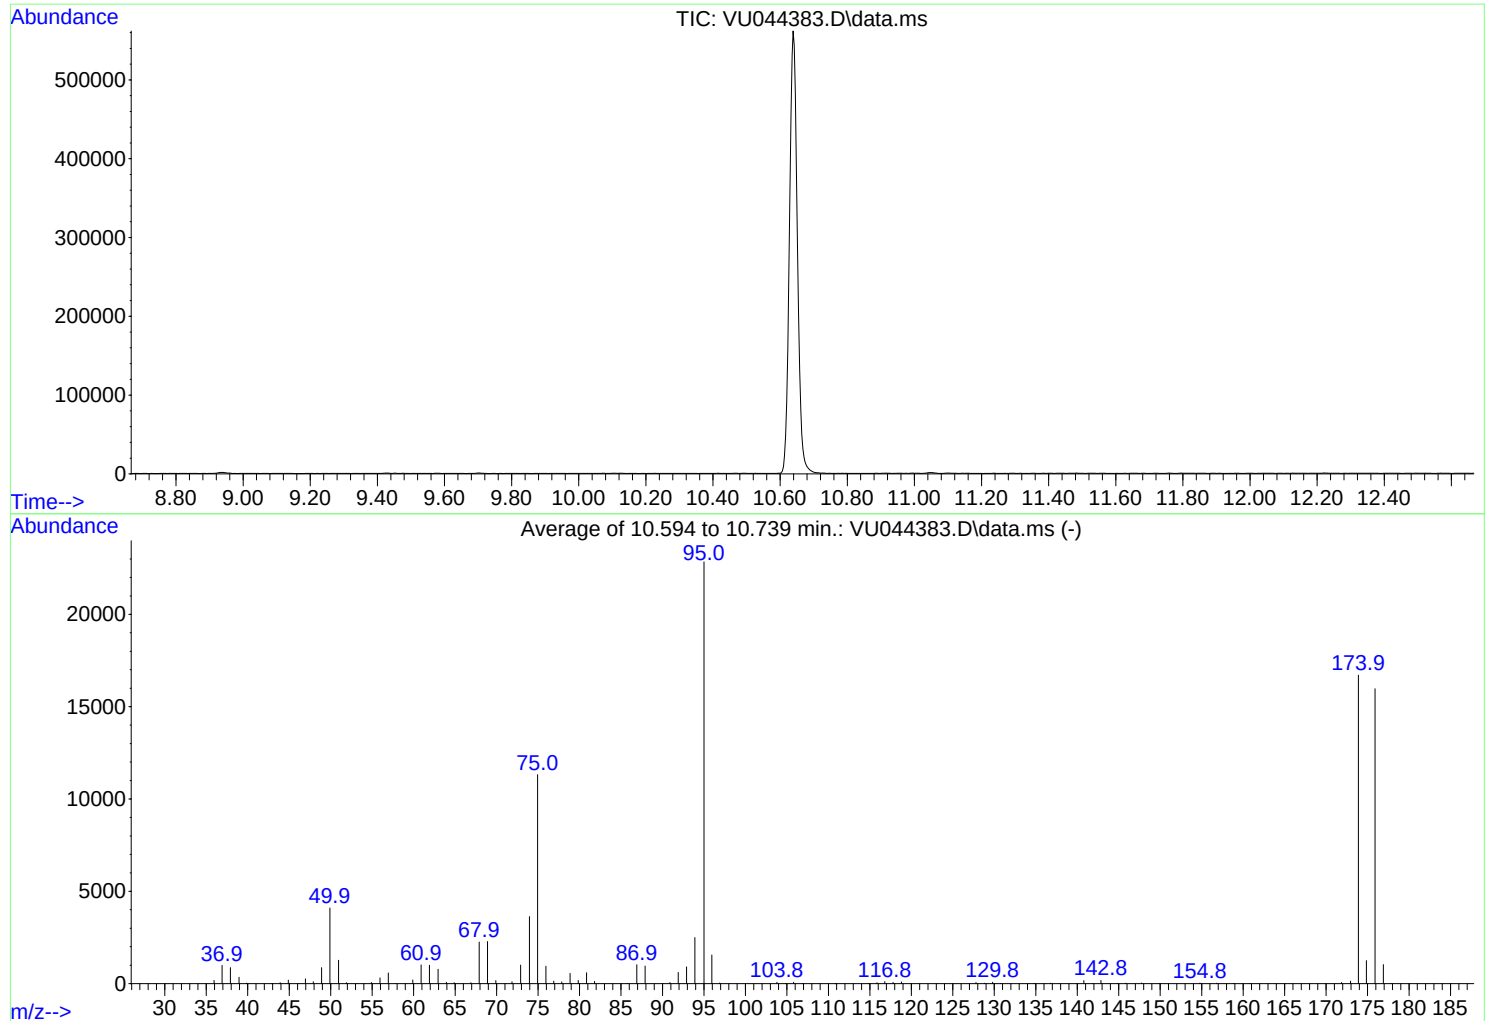

AutoFind: Averaged scan 2878 to 2923; Bkg corrected with scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	4099	PASS
75	95	30	60	49.5	11317	PASS
95	95	100	100	100.0	22844	PASS
96	95	5	9	6.8	1548	PASS
173	174	0.00	2	0.8	135	PASS
174	95	50	100	73.1	16703	PASS
175	174	5	9	7.5	1246	PASS
176	174	95	101	95.6	15969	PASS
177	176	5	9	6.5	1032	PASS