

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072222\
 Data File : VU049858.D
 Acq On : 22 Jul 2022 18:38
 Operator : SY/MD
 Sample : N3802-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBHY2

Quant Time: Jul 23 02:36:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 23 01:04:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	89395	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	86597	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	36460	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	37635	5.200	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	104.000%	
7) Chloroethane-d5	1.909	69	32707	5.400	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.000%	
11) 1,1-Dichloroethene-d2	2.565	65	16663	5.158	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	103.200%	
20) 2-Butanone-d5	4.636	46	117279	45.037	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	90.080%	
24) Chloroform-d	5.063	84	82883	5.142	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.800%	
26) 1,2-Dichloroethane-d4	5.703	65	48261	5.106	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.200%	
32) Benzene-d6	5.729	84	153050	5.187	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.800%	
36) 1,2-Dichloropropane-d6	6.690	67	54560	5.352	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	107.000%	
41) Toluene-d8	7.899	98	124256	4.817	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	8.179	79	17601	4.755	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.200%	
46) 2-Hexanone-d5	8.639	63	81101	55.297	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	110.600%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	43623	5.096	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	102.000%	
66) 1,2-Dichlorobenzene-d4	12.195	152	41792	5.553	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.000%	
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.385	85	14684	1.556	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072222\
Data File : VU049858.D
Acq On : 22 Jul 2022 18:38
Operator : SY/MD
Sample : N3802-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBHY2

Quant Time: Jul 23 02:36:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 23 01:04:38 2022
Response via : Initial Calibration

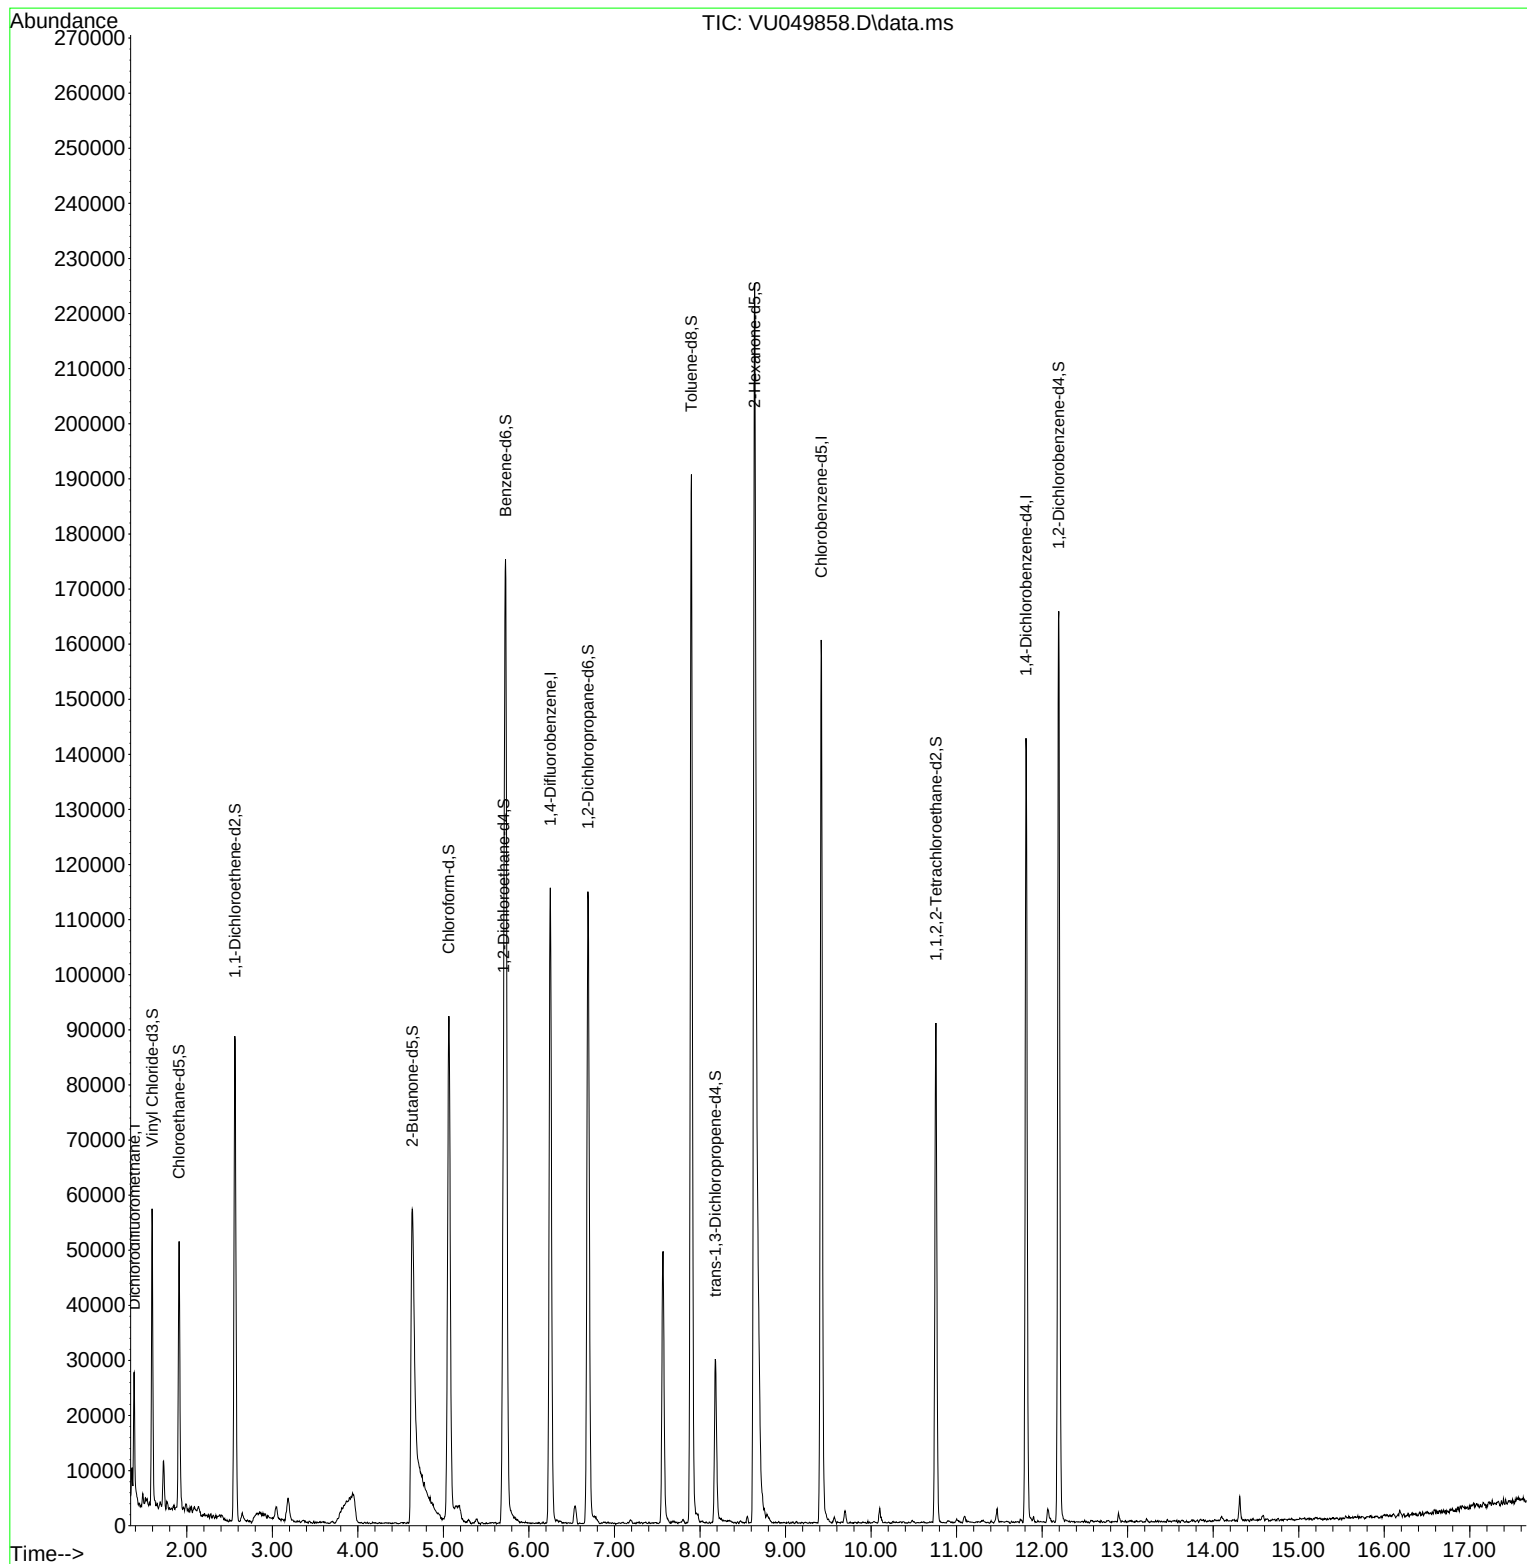

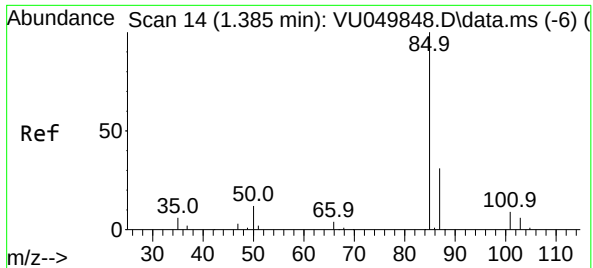

#2
 Dichlorodifluoromethane
 Concen: 1.556 ug/L
 RT: 1.385 min Scan# 14
 Delta R.T. 0.000 min
 Lab File: VU049858.D
 Acq: 22 Jul 2022 18:38

Instrument :
 MSVOA_U
 ClientSampleId :
 GBHY2

Tgt Ion: 85 Resp: 14684
 Ion Ratio Lower Upper
 85 100
 87 31.0 25.4 38.2

