
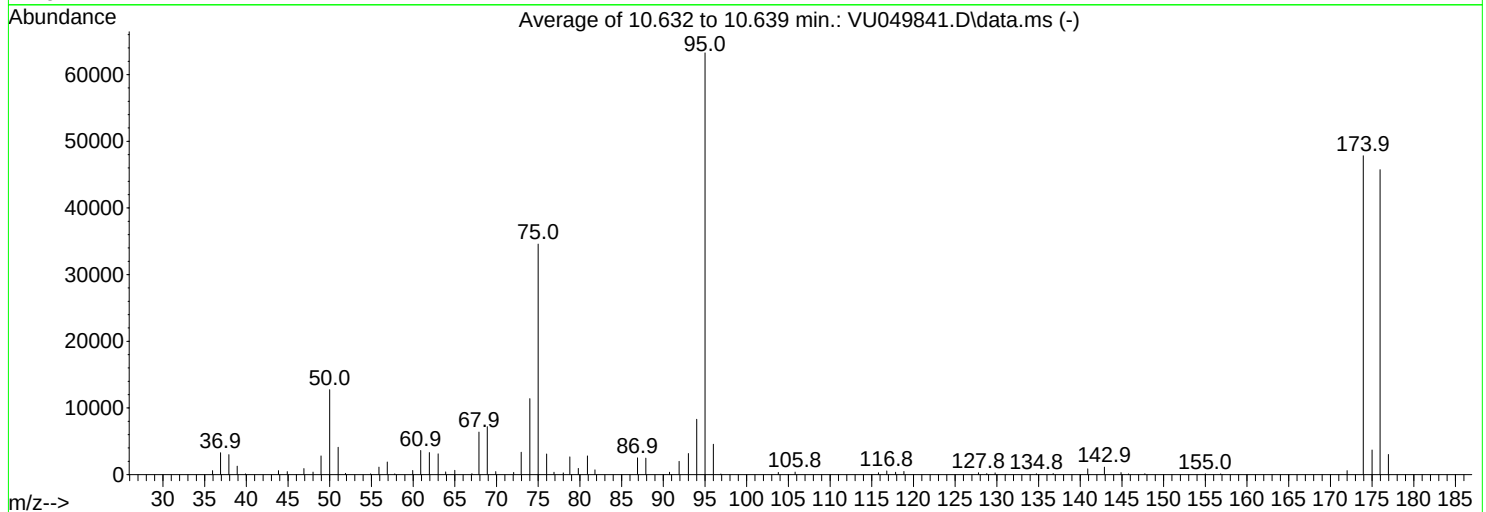


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072222\
 Data File : VU049841.D
 Acq On : 22 Jul 2022 08:44
 Operator : SY/MD
 Sample : BFB092
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB092

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jul 23 01:04:38 2022

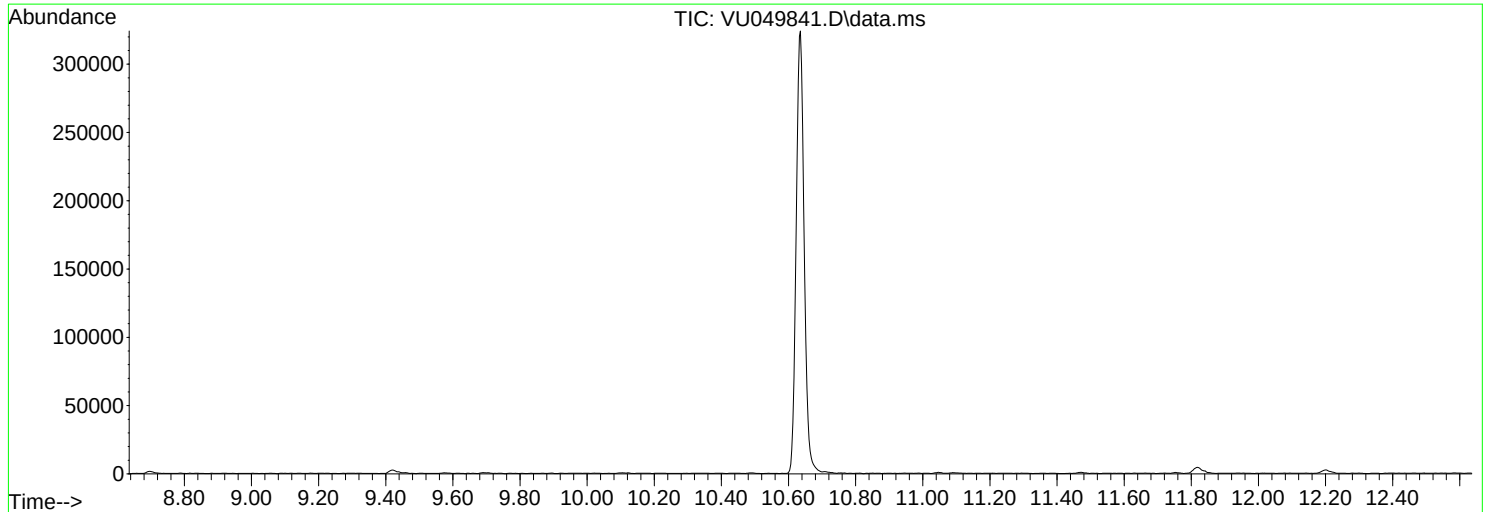

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	12752	PASS
75	95	30	80	54.7	34587	PASS
95	95	100	100	100.0	63267	PASS
96	95	5	9	7.2	4561	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.6	47821	PASS
175	174	5	9	7.7	3689	PASS
176	174	95	101	95.7	45755	PASS
177	176	5	9	6.6	3039	PASS

m/z	Abundance
39.90	139.0
43.80	243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
35.90	630.0
36.90	3202.0
37.90	3228.0
38.90	1391.0
39.90	312.0
43.90	952.0
44.90	455.0
46.00	118.0
46.90	848.0
48.00	401.0
48.90	3024.0
50.00	13205.0
51.00	4317.0
51.90	178.0
54.90	133.0
55.90	1238.0
56.90	1933.0
57.80	133.0
59.90	644.0
60.90	3719.0
62.00	3565.0
63.00	3091.0
63.90	434.0
65.00	672.0
67.00	158.0
67.90	6593.0
68.90	7289.0
69.90	471.0
72.10	323.0
72.90	3433.0
74.00	11641.0
75.00	35640.0
76.00	3159.0
76.90	462.0
78.00	272.0
78.80	2784.0
79.80	961.0
80.90	2881.0
81.80	674.0
86.90	2583.0
87.90	2545.0
90.70	333.0
91.90	2068.0
93.00	3324.0
94.00	8548.0
95.00	64672.0
96.00	4627.0
96.90	168.0
103.80	261.0
105.80	422.0
115.80	288.0
116.80	563.0
117.90	353.0
118.90	542.0
127.80	273.0
128.80	144.0
129.80	327.0
134.80	154.0
136.80	187.0
140.90	884.0
142.90	1058.0
144.90	342.0
145.80	150.0
147.80	168.0
155.00	112.0
156.90	110.0
172.00	562.0
174.00	47504.0
175.00	3721.0
175.90	45856.0
176.90	3009.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
36.00	605.0
36.90	3448.0
37.90	3087.0
38.90	1298.0
39.90	291.0
43.90	862.0
44.90	467.0
46.90	954.0
48.00	406.0
49.00	2861.0
50.00	13087.0
51.00	4275.0
51.90	194.0
54.90	120.0
55.90	1175.0
56.90	1931.0
57.80	129.0
59.90	626.0
60.90	3755.0
62.00	3412.0
63.00	3272.0
63.90	421.0
65.00	678.0
67.10	143.0
67.90	6573.0
68.90	7428.0
69.90	485.0
72.10	357.0
73.00	3458.0
74.00	11696.0
75.00	35504.0
76.00	3244.0
76.90	384.0
78.00	281.0
78.80	2709.0
79.80	976.0
80.90	2846.0
81.80	751.0
86.90	2587.0
87.90	2612.0
90.80	370.0
91.90	2047.0
93.00	3308.0
94.00	8639.0
95.00	65256.0
96.00	4753.0
96.90	139.0
103.80	338.0
105.80	415.0
115.80	309.0
116.80	571.0
117.80	377.0
118.90	493.0
127.80	303.0
128.80	171.0
129.80	270.0
134.80	157.0
136.80	183.0
140.90	877.0
142.90	1170.0
144.90	319.0
145.80	139.0
147.70	161.0
155.00	142.0
156.80	135.0
172.00	583.0
173.90	49192.0
175.00	3837.0
176.00	47128.0
177.00	3098.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
36.00	548.0
36.90	3231.0
37.90	2729.0
38.90	1129.0
39.90	216.0
43.90	720.0
44.90	455.0
46.90	948.0
48.00	371.0
48.90	2541.0
50.00	11964.0
51.00	3765.0
51.90	179.0
54.90	133.0
55.90	975.0
56.90	1824.0
57.80	121.0
60.00	602.0
60.90	3377.0
61.90	2954.0
63.00	2994.0
63.90	369.0
65.00	592.0
67.00	123.0
67.90	5966.0
68.90	6877.0
69.90	399.0
71.90	347.0
73.00	3211.0
74.00	10899.0
75.00	32616.0
76.00	2914.0
76.90	270.0
78.00	251.0
78.80	2537.0
79.80	874.0
80.90	2697.0
81.80	734.0
86.90	2368.0
87.90	2304.0
90.80	369.0
91.90	1881.0
93.00	2869.0
94.00	7751.0
95.00	59872.0
96.00	4304.0
103.80	390.0
105.80	330.0
115.80	310.0
116.80	555.0
117.80	336.0
118.80	395.0
127.80	288.0
128.80	167.0
129.80	220.0
131.10	121.0
134.70	139.0
136.70	165.0
140.90	841.0
142.90	1160.0
144.90	263.0
145.80	108.0
147.70	127.0
155.00	135.0
156.80	138.0
172.00	634.0
173.90	46768.0
175.00	3508.0
176.00	44280.0
177.00	3009.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092