


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072223\
Data File : VU054840.D
Acq On : 21 Jul 2023 16:03
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072123DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Mon Jul 24 09:59:15 2023

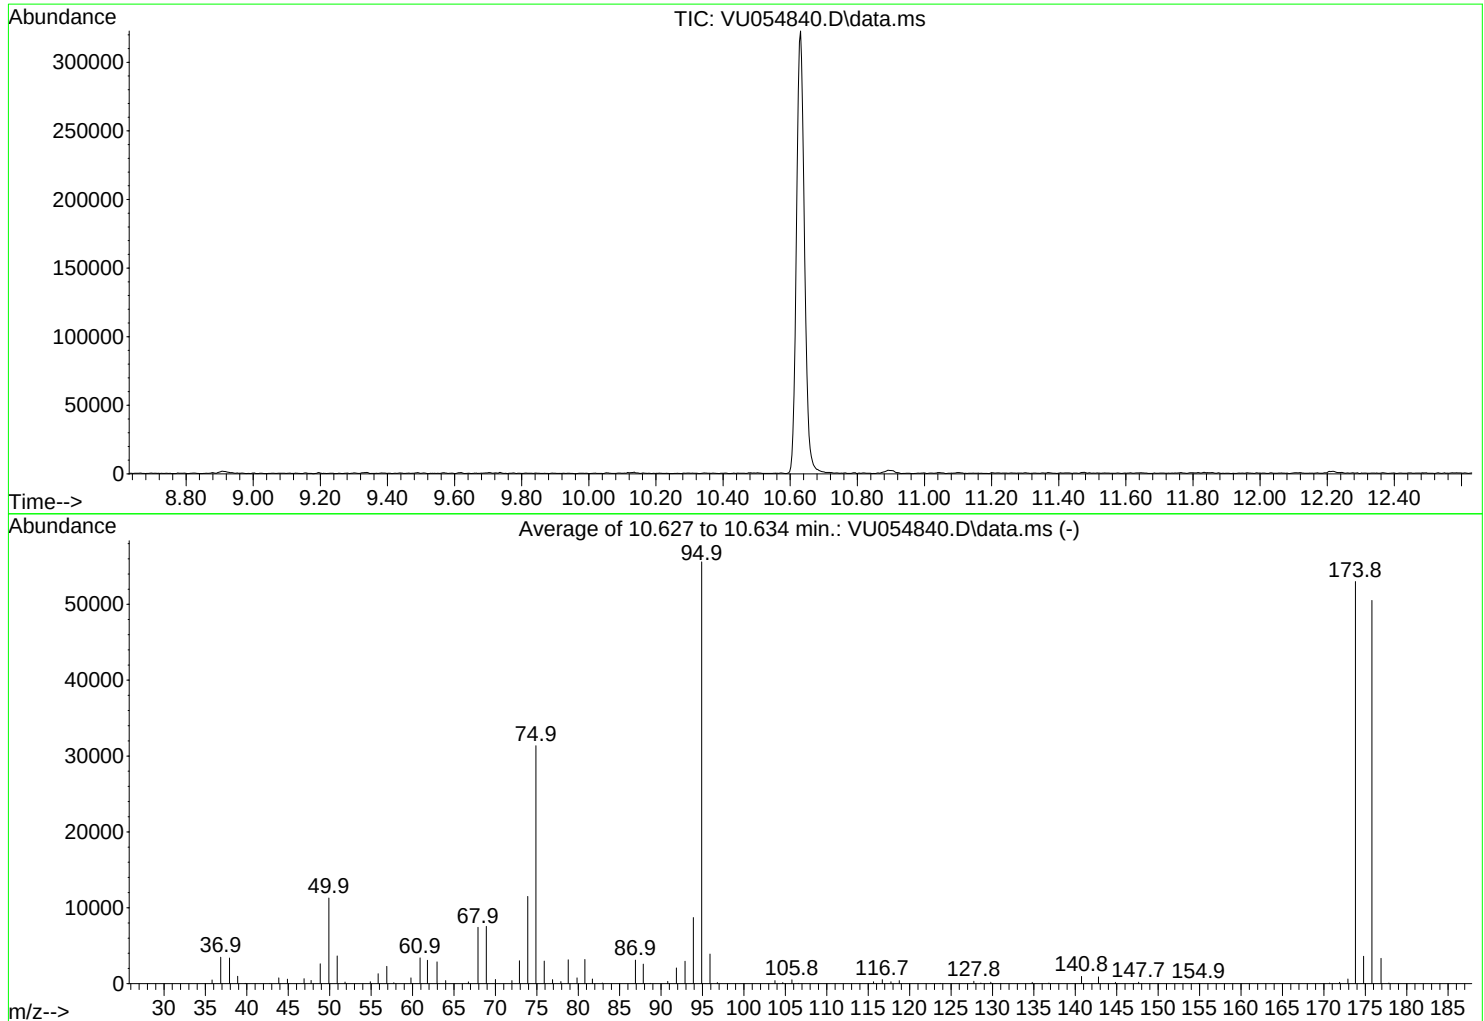

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	11283	PASS
75	95	30	60	56.4	31363	PASS
95	95	100	100	100.0	55600	PASS
96	95	5	9	7.0	3894	PASS
173	174	0.00	2	1.2	614	PASS
174	95	50	100	95.3	53000	PASS
175	174	5	9	6.8	3610	PASS
176	174	95	101	95.3	50509	PASS
177	176	5	9	6.6	3329	PASS