


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072318\
Data File : VU025595.D
Acq On : 23 Jul 2018 10:13
Operator : MD/SY
Sample : BFB48
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Title : VOC Analysis
Last Update : Sat Aug 04 04:39:04 2018

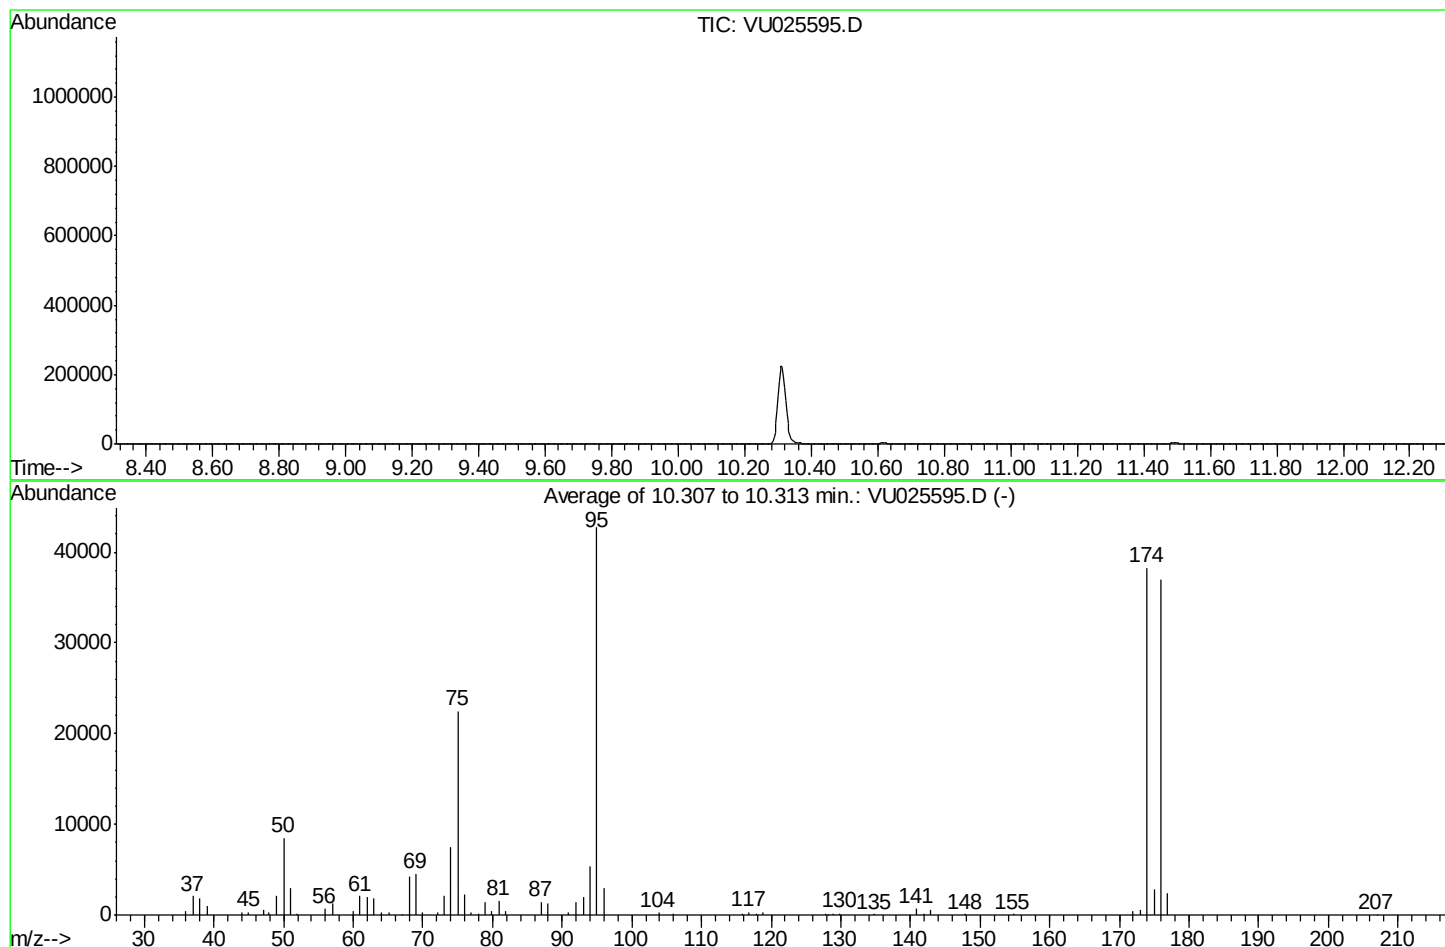

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8470	PASS
75	95	30	80	52.7	22504	PASS
95	95	100	100	100.0	42730	PASS
96	95	5	9	6.8	2919	PASS
173	174	0.00	2	1.4	521	PASS
174	95	50	120	89.6	38269	PASS
175	174	5	9	7.3	2795	PASS
176	174	95	101	96.6	36962	PASS
177	176	5	9	6.5	2400	PASS

m/z	Abundance
39.90	116.0
44.00	390.0
207.00	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	298.0
37.00	2007.0
38.00	2010.0
39.00	922.0
39.90	127.0
44.00	699.0
45.00	330.0
47.10	503.0
47.90	273.0
49.00	2221.0
50.00	8462.0
51.00	2823.0
51.90	127.0
55.90	660.0
57.00	1213.0
60.10	365.0
61.00	2113.0
62.00	1964.0
63.00	1949.0
63.90	231.0
65.10	267.0
68.00	4328.0
69.00	4670.0
69.90	278.0
72.00	265.0
73.00	2139.0
74.00	7359.0
75.00	22408.0
76.00	2332.0
76.80	252.0
78.00	172.0
78.90	1409.0
79.90	508.0
80.90	1597.0
81.90	408.0
87.00	1418.0
87.90	1371.0
90.90	237.0
92.00	1271.0
93.00	1913.0
94.00	5148.0
95.00	41184.0
96.00	3008.0
103.80	219.0
105.80	196.0
115.90	180.0
116.90	262.0
117.80	141.0
118.80	247.0
128.10	116.0
128.90	110.0
129.90	226.0
134.80	110.0
140.90	611.0
141.90	112.0
142.90	474.0
154.80	133.0
172.00	386.0
173.00	489.0
174.00	36464.0
175.00	2692.0
176.00	34840.0
176.90	2301.0
206.90	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	402.0
37.00	2160.0
38.00	1889.0
39.00	943.0
39.90	102.0
43.90	606.0
45.00	307.0
47.10	579.0
47.90	320.0
49.00	2151.0
50.00	8733.0
51.00	3128.0
51.90	109.0
56.00	709.0
57.00	1279.0
60.00	438.0
61.00	2166.0
62.00	2071.0
63.00	1959.0
63.90	231.0
65.10	248.0
68.00	4292.0
69.00	4711.0
70.00	295.0
72.10	324.0
73.00	2176.0
74.00	7751.0
75.00	23096.0
76.00	2360.0
76.80	263.0
78.00	207.0
78.90	1484.0
79.90	478.0
80.90	1640.0
81.90	469.0
86.90	1501.0
87.90	1355.0
90.80	279.0
92.00	1542.0
93.00	2021.0
94.00	5610.0
95.00	44056.0
96.00	2960.0
103.80	222.0
105.80	207.0
115.90	184.0
116.80	340.0
117.80	176.0
118.80	247.0
127.80	141.0
128.90	126.0
129.90	188.0
134.80	125.0
140.90	681.0
141.90	136.0
142.90	540.0
147.90	115.0
154.80	125.0
172.00	447.0
173.00	519.0
174.00	39440.0
174.90	2831.0
176.00	38160.0
177.00	2480.0
206.90	261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	461.0
37.00	2102.0
38.00	1653.0
39.00	914.0
43.90	598.0
45.00	321.0
47.00	527.0
47.90	318.0
49.00	1845.0
50.00	8216.0
51.00	3028.0
56.00	647.0
57.00	1225.0
60.00	483.0
61.00	1926.0
62.00	1941.0
63.00	1737.0
64.00	192.0
65.00	244.0
67.00	114.0
68.00	3989.0
69.00	4355.0
70.00	311.0
72.10	294.0
73.00	1943.0
74.00	7348.0
75.00	22008.0
76.00	2055.0
76.90	298.0
77.90	223.0
78.90	1435.0
79.90	431.0
80.90	1492.0
81.90	447.0
86.90	1487.0
88.00	1260.0
90.80	295.0
92.00	1599.0
93.00	2021.0
94.00	5411.0
95.00	42952.0
96.00	2790.0
103.90	238.0
105.90	210.0
115.90	185.0
116.80	355.0
117.80	213.0
118.80	209.0
127.80	211.0
128.80	104.0
129.90	151.0
134.80	118.0
140.90	647.0
141.90	143.0
142.90	568.0
147.90	156.0
171.90	442.0
173.00	556.0
174.00	38904.0
174.90	2864.0
176.00	37888.0
177.00	2420.0
207.00	257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48