

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072319\
Data File : VU033369.D
Acq On : 23 Jul 2019 09:34
Operator : JC/SP
Sample : VU0723WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0723WBL01

Quant Time: Jul 24 02:47:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U072219DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jul 23 03:43:51 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.72	96	29866	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.30	95	9435	0.80	ug/l	0.00
Spiked Amount	1.000		Recovery	=	80.00%	
68) 1,2-Dichlorobenzene-d4	11.85	152	10020	0.83	ug/l	0.00
Spiked Amount	1.000		Recovery	=	83.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072319\
Data File : VU033369.D
Acq On : 23 Jul 2019 09:34
Operator : JC/SP
Sample : VU0723WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0723WBL01

Quant Time: Jul 24 02:47:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U072219DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jul 23 03:43:51 2019
Response via : Initial Calibration

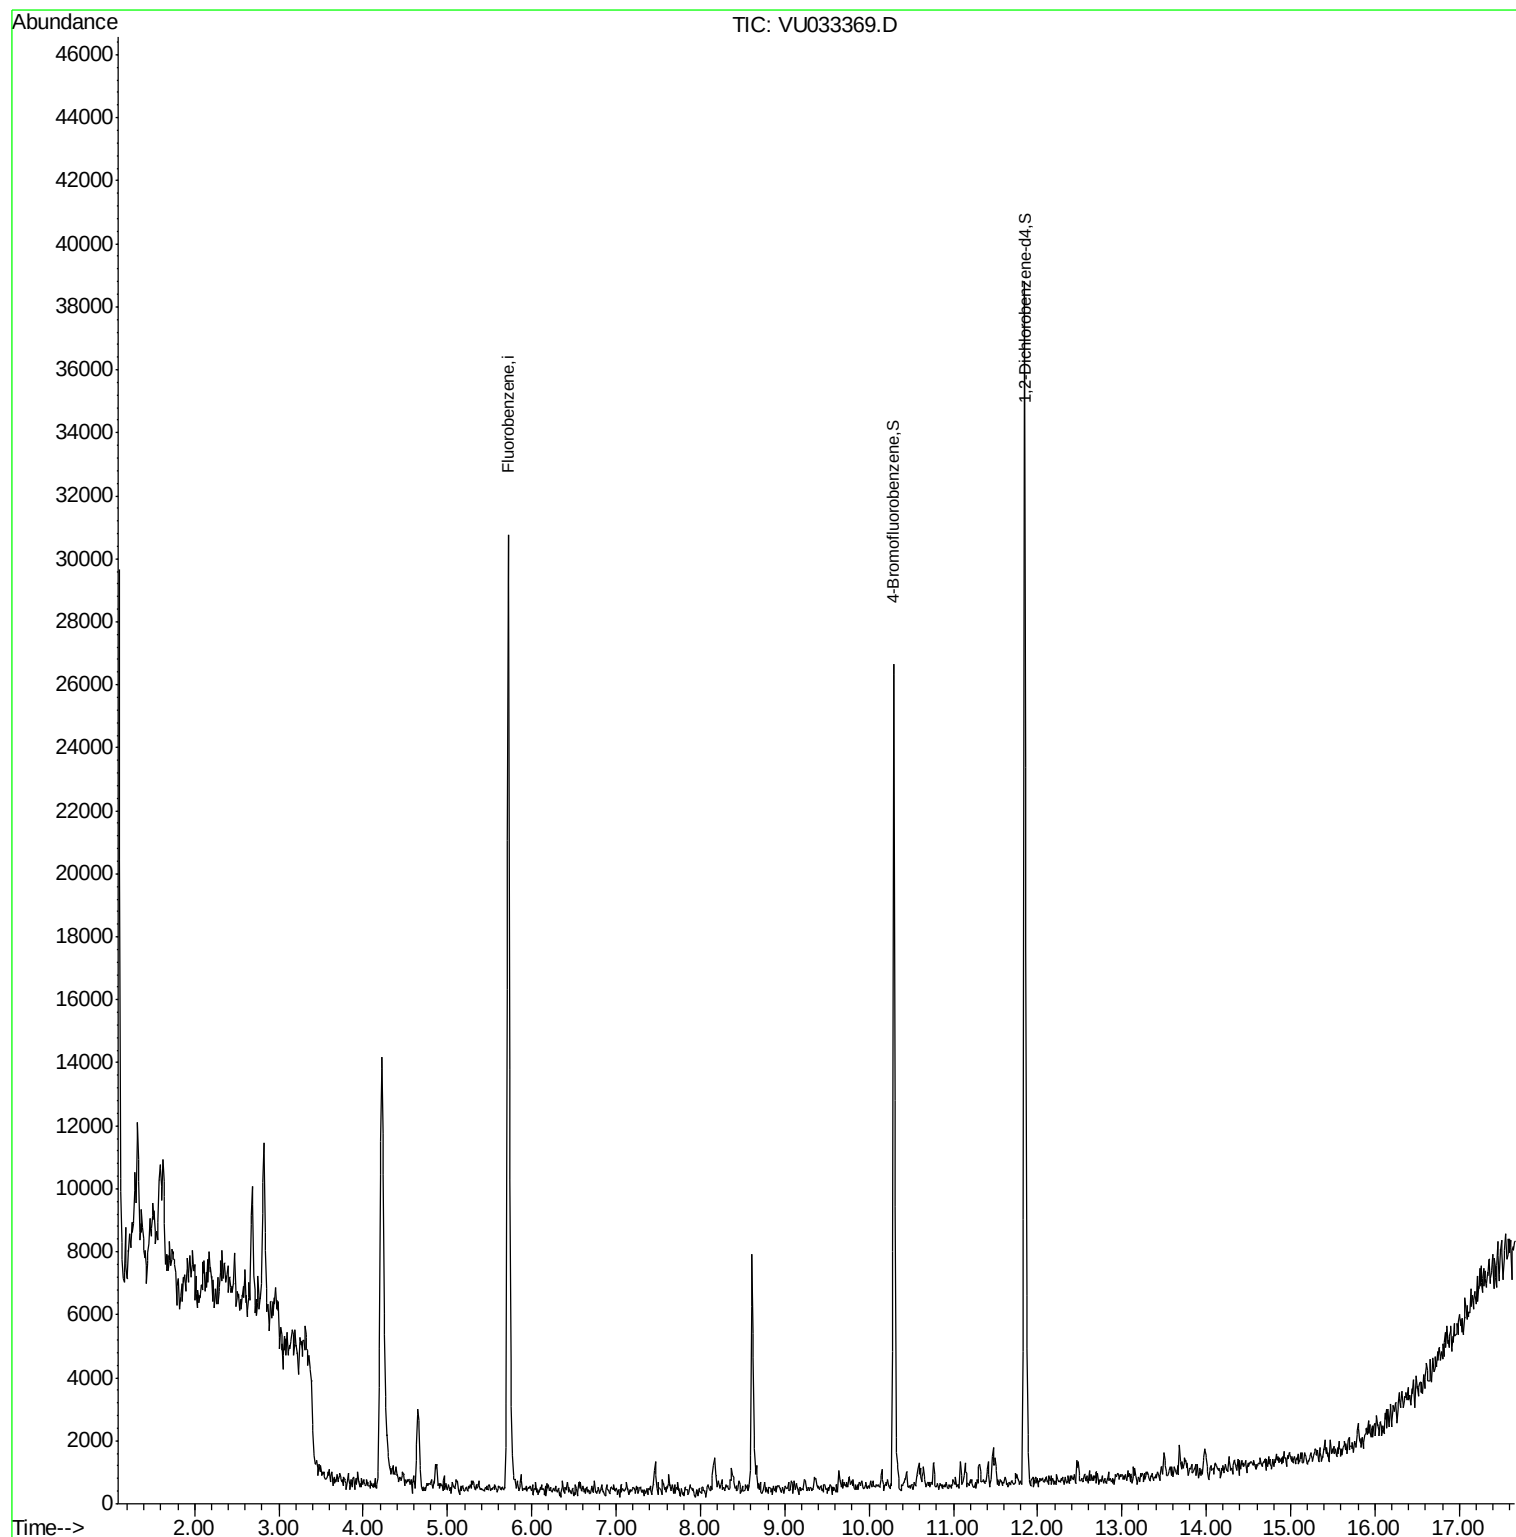

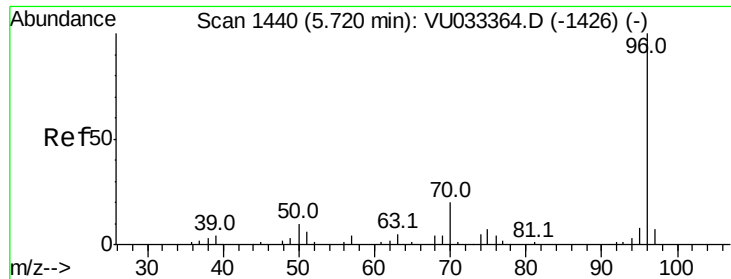

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.72 min Scan# 1441

Delta R.T. 0.00 min

Lab File: VU033369.D

Acq: 23 Jul 2019 09:34

Instrument :

MSVOA_U

ClientSampleId :

VU0723WBL01

Tot Ion: 96 Resp: 29866


Ion Ratio Lower Upper

96 100

70 19.7 16.4 24.6

95 8.8 6.7 10.1

97 5.6 0.0 0.0#



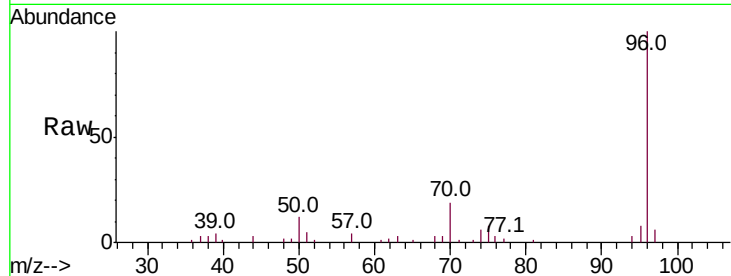


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

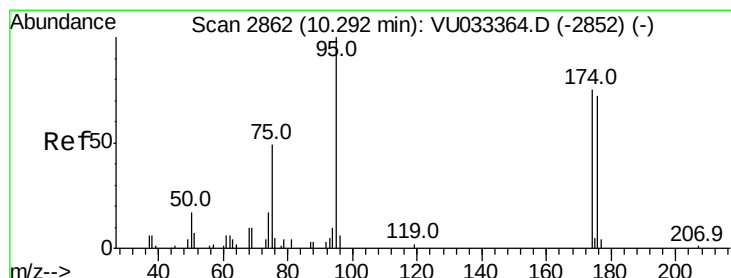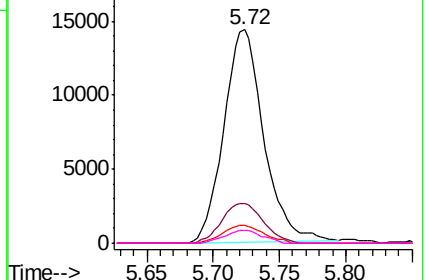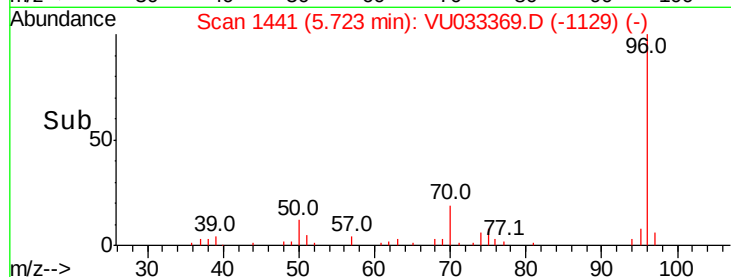

#57

4-Bromofluorobenzene

Concen: 0.805 ug/l

RT: 10.30 min Scan# 2863

Delta R.T. 0.00 min

Lab File: VU033369.D

Acq: 23 Jul 2019 09:34


Tgt Ion: 95 Resp: 9435

Ion Ratio Lower Upper

95 100

174 77.5 58.8 88.2



176 72.8 54.4 81.6

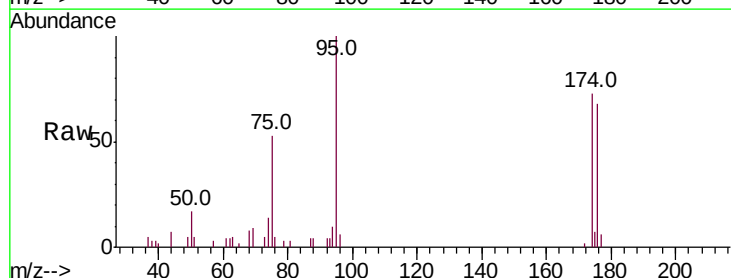


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

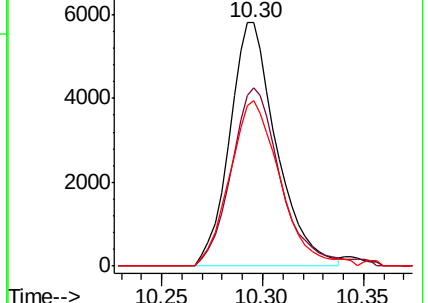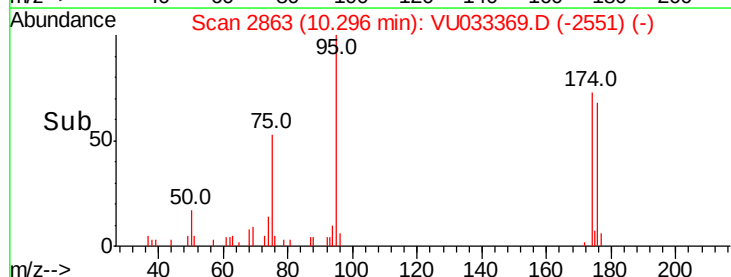

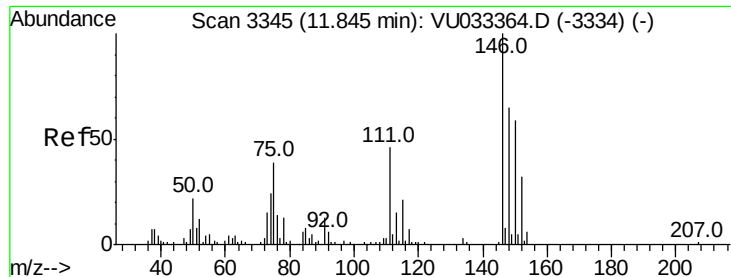

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.828 ug/l
 RT: 11.85 min Scan# 3346
 Delta R.T. 0.00 min
 Lab File: VU033369.D
 Acq: 23 Jul 2019 09:34

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0723WBL01

Tot Ion:152 Resp: 10020
 Ion Ratio Lower Upper
 152 100
 115 70.4 0.0 123.2
 150 165.1 0.0 648.4

