


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072319\
Data File : VU033367.D
Acq On : 23 Jul 2019 08:23
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072219DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Jul 24 03:53:19 2019

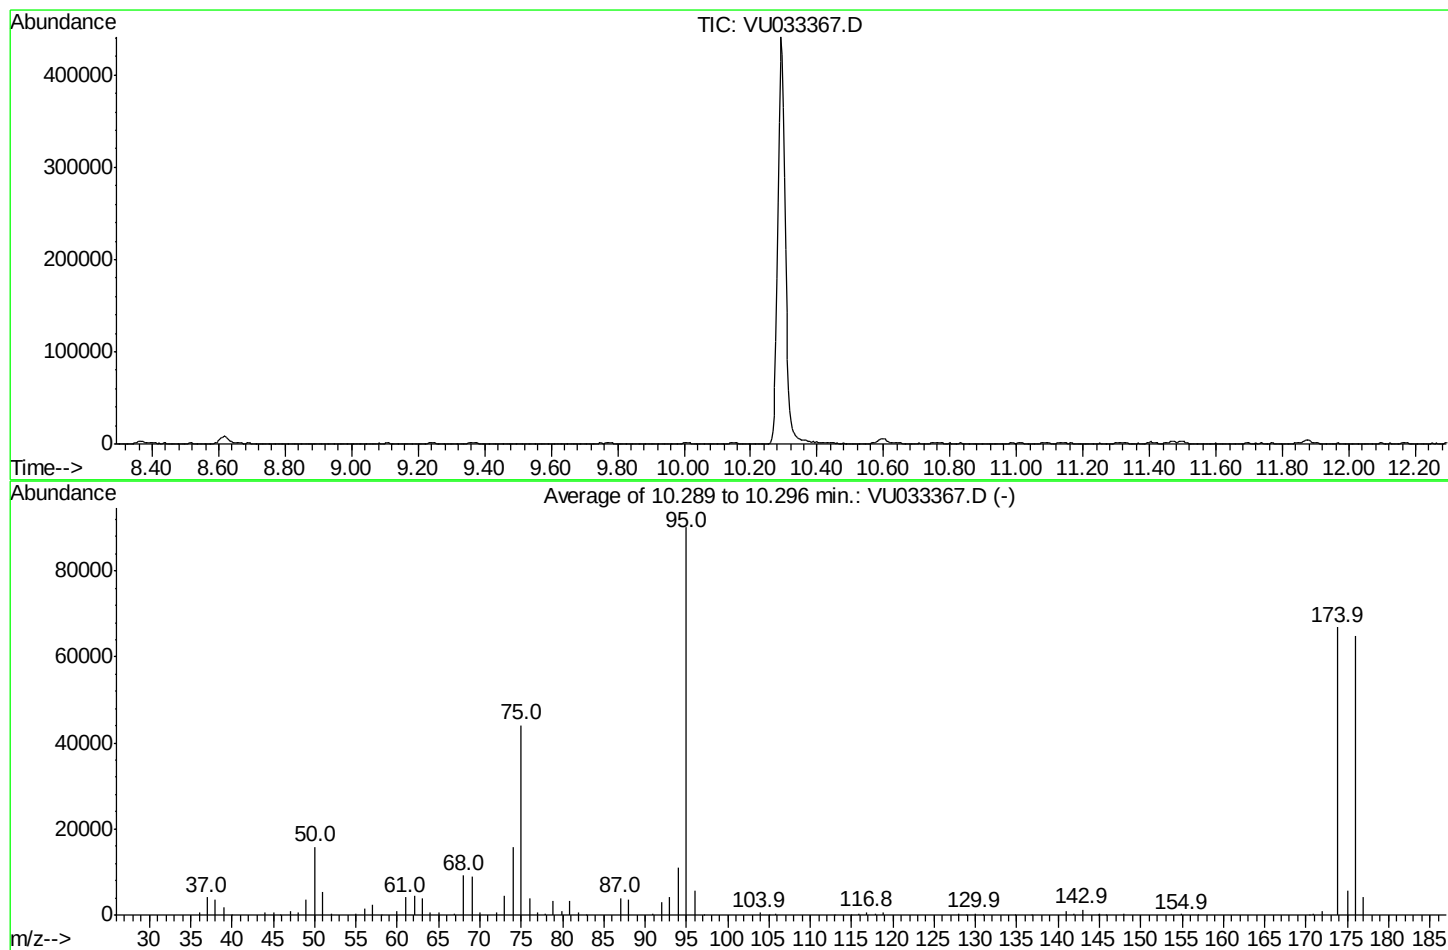

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	15899	PASS
75	95	30	60	49.0	44168	PASS
95	95	100	100	100.0	90122	PASS
96	95	5	9	6.4	5794	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.2	66904	PASS
175	174	5	9	8.2	5518	PASS
176	174	95	101	97.2	65000	PASS
177	176	5	9	6.4	4183	PASS