


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072320\
 Data File : VU039630.D
 Acq On : 23 Jul 2020 10:23
 Operator : SY/MD
 Sample : BFB51
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072320WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 24 03:50:28 2020

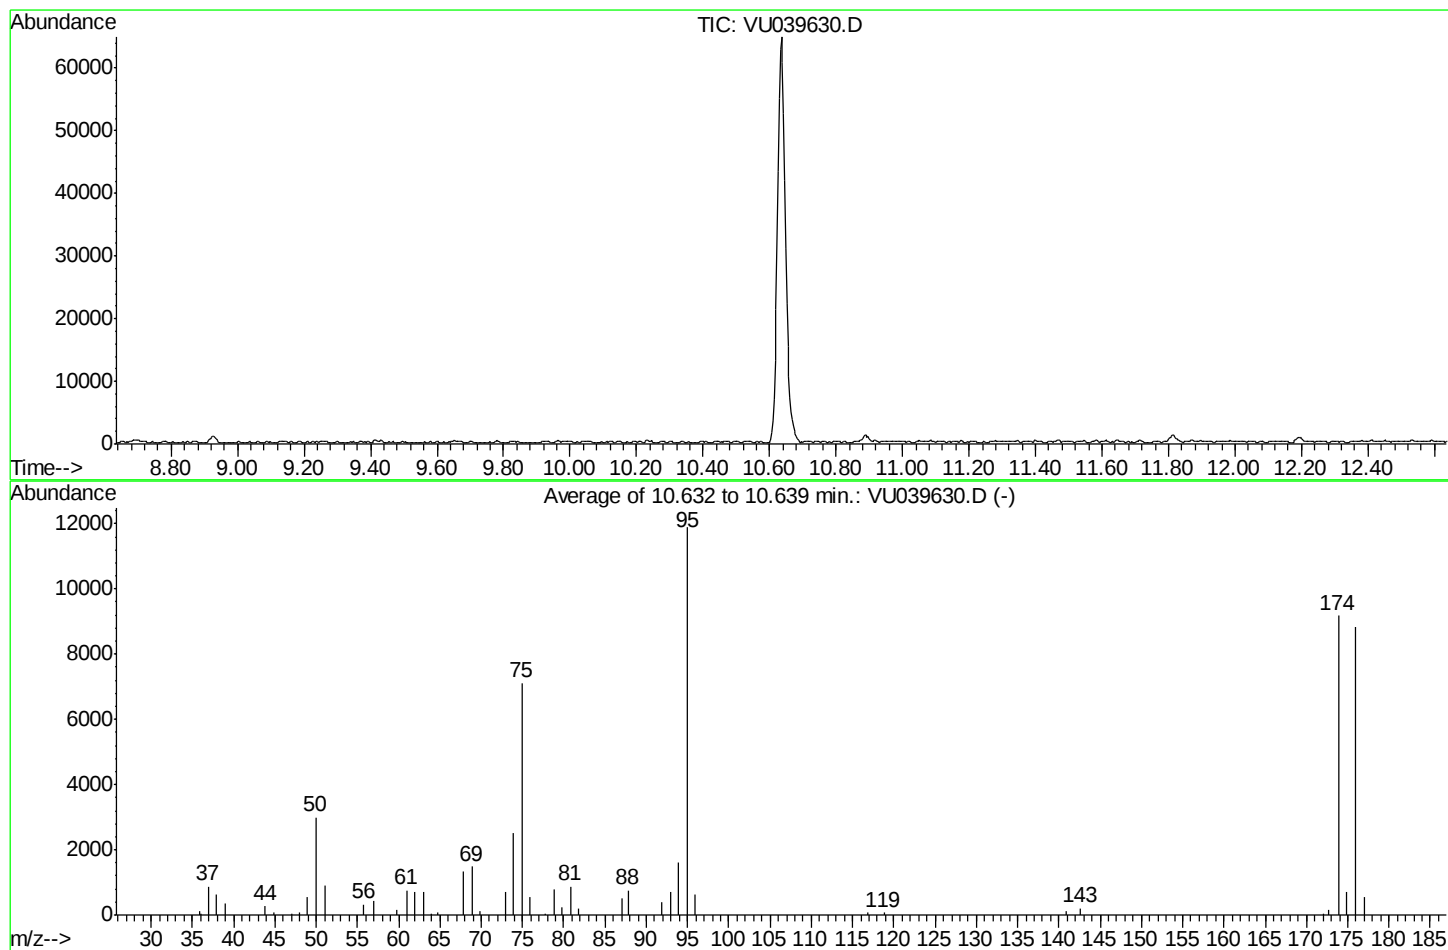

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.2	2998	PASS
75	95	30	80	59.8	7105	PASS
95	95	100	100	100.0	11888	PASS
96	95	5	9	5.4	642	PASS
173	174	0.00	2	1.9	170	PASS
174	95	50	120	77.2	9180	PASS
175	174	5	9	7.8	720	PASS
176	174	95	101	96.4	8851	PASS
177	176	5	9	6.2	547	PASS

m/z	Abundance
35.80	198.0
36.90	755.0
38.00	676.0
38.90	378.0
43.90	412.0
47.00	111.0
47.90	140.0
48.90	625.0
49.90	3002.0
51.00	1004.0
55.80	335.0
57.00	481.0
59.80	197.0
61.00	777.0
62.00	741.0
63.00	704.0
67.90	1413.0
68.90	1518.0
70.00	101.0
72.90	697.0
74.00	2658.0
74.90	7148.0
75.90	557.0
77.70	118.0
78.90	793.0
79.80	258.0
80.80	846.0
81.80	192.0
87.00	568.0
87.80	648.0
91.90	364.0
93.00	698.0
94.00	1755.0
95.00	11966.0
95.90	632.0
116.80	113.0
118.80	125.0
140.90	137.0
142.70	241.0
172.70	159.0
173.90	8839.0
174.90	726.0
175.90	8720.0
177.00	478.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
35.80	176.0
36.90	899.0
37.90	615.0
39.00	377.0
43.90	492.0
44.90	102.0
47.90	114.0
48.90	586.0
50.00	3155.0
51.00	943.0
55.80	348.0
57.00	458.0
59.80	193.0
60.90	793.0
62.00	729.0
62.90	724.0
63.90	100.0
64.80	134.0
67.90	1365.0
68.90	1558.0
69.90	116.0
73.00	722.0
73.90	2611.0
74.90	7377.0
76.00	556.0
78.90	840.0
79.80	259.0
80.80	900.0
81.80	204.0
87.00	548.0
87.80	833.0
91.90	418.0
93.00	747.0
94.00	1616.0
95.00	12185.0
95.90	656.0
116.80	113.0
118.80	103.0
140.90	147.0
142.60	214.0
172.70	181.0
173.90	9412.0
174.90	752.0
175.90	9056.0
176.90	555.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	156.0
36.90	988.0
37.90	560.0
39.00	279.0
43.90	507.0
44.90	106.0
48.90	500.0
50.00	2838.0
51.00	807.0
55.80	270.0
57.00	407.0
59.70	139.0
60.90	714.0
61.90	665.0
62.90	669.0
64.80	139.0
67.90	1287.0
68.90	1386.0
69.80	142.0
73.00	723.0
73.90	2274.0
75.00	6790.0
76.00	524.0
78.90	750.0
79.80	230.0
80.90	878.0
81.90	193.0
87.00	456.0
87.80	761.0
91.90	443.0
92.90	705.0
93.90	1495.0
95.00	11514.0
95.90	638.0
140.90	111.0
142.60	151.0
172.00	140.0
172.70	171.0
173.90	9291.0
174.90	683.0
175.90	8779.0
176.90	610.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
43.70	194.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51