
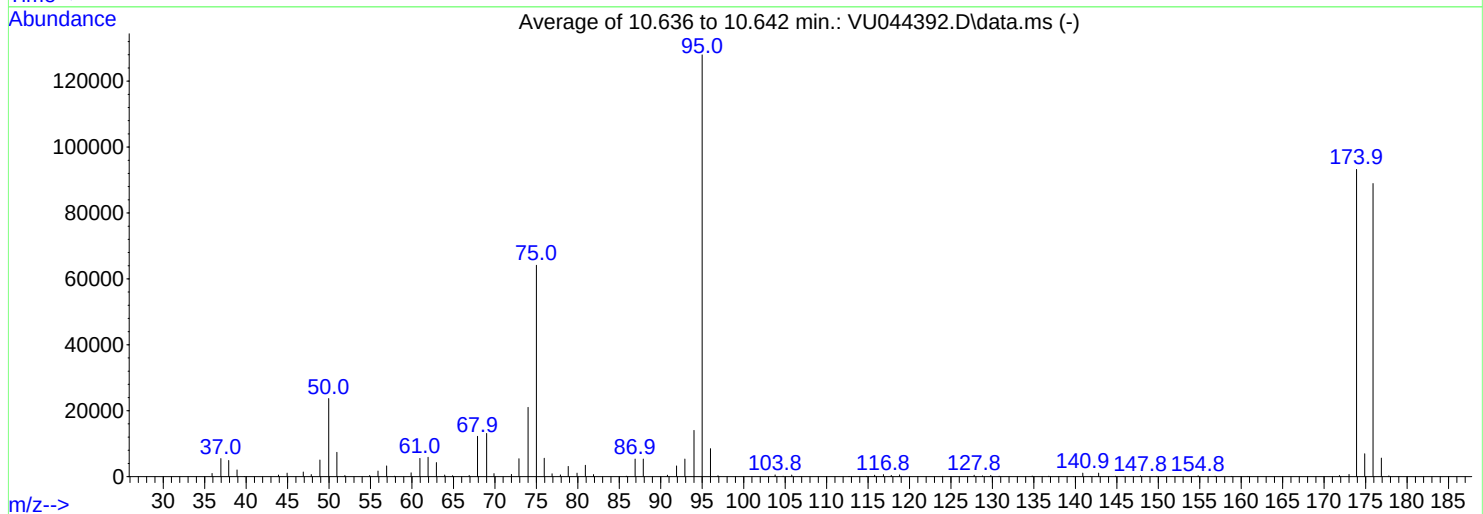


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072321\
 Data File : VU044392.D
 Acq On : 23 Jul 2021 08:59
 Operator : SY/MD
 Sample : BFB003
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB003

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jul 24 01:01:20 2021

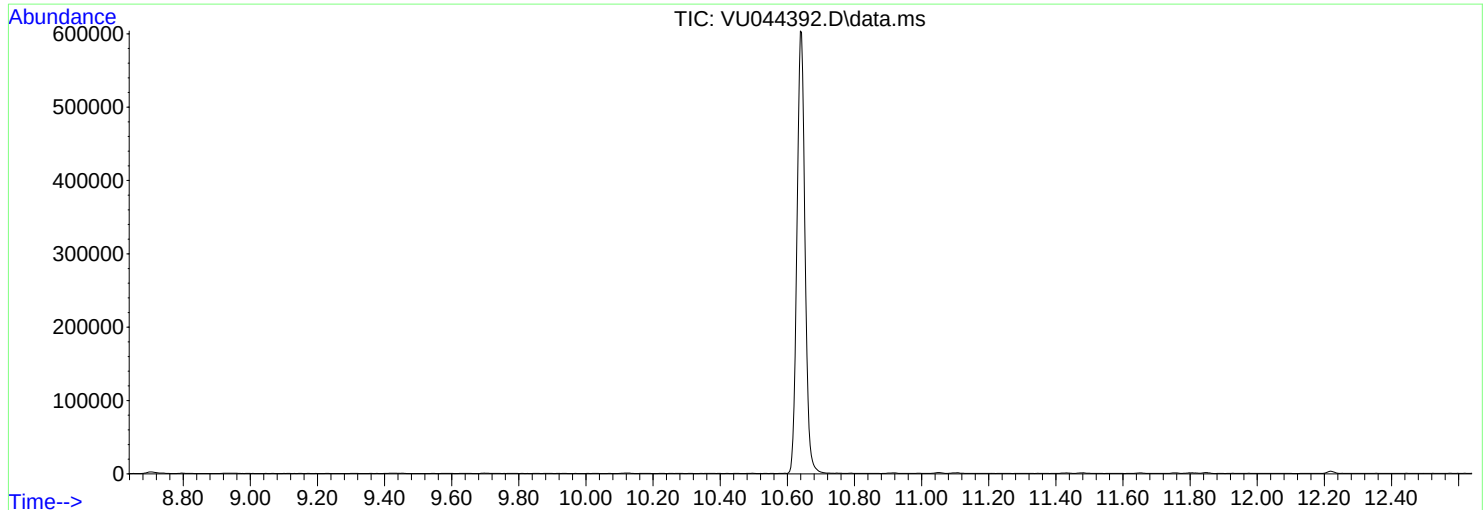

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	23685	PASS
75	95	30	80	50.1	64131	PASS
95	95	100	100	100.0	127984	PASS
96	95	5	9	6.7	8515	PASS
173	174	0.00	2	0.7	666	PASS
174	95	50	120	72.8	93224	PASS
175	174	5	9	7.4	6940	PASS
176	174	95	101	95.4	88947	PASS
177	176	5	9	6.4	5651	PASS

m/z	Abundance
39.80	135.0
43.90	665.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.90	916.0
36.90	5352.0
37.90	4633.0
38.90	1985.0
39.80	206.0
43.90	1115.0
44.90	1070.0
46.90	1339.0
47.80	637.0
48.90	4683.0
49.90	22704.0
51.00	7137.0
51.90	320.0
54.90	302.0
55.90	1567.0
57.00	3264.0
57.90	163.0
59.90	1072.0
61.00	5338.0
61.90	5642.0
63.00	4166.0
63.90	457.0
64.90	296.0
66.90	314.0
67.90	11777.0
69.00	12390.0
69.90	907.0
72.00	682.0
72.90	5025.0
74.00	20032.0
75.00	61328.0
75.90	5457.0
76.90	926.0
77.90	464.0
78.80	3004.0
79.90	988.0
80.90	3217.0
81.90	597.0
85.90	132.0
86.90	5119.0
87.90	4956.0
90.80	397.0
91.90	3104.0
92.90	5027.0
94.00	13414.0
95.00	121280.0
96.00	8247.0
96.90	266.0
103.80	490.0
104.80	161.0
105.80	481.0
106.80	102.0
114.80	104.0
115.80	416.0
116.80	670.0
117.80	372.0
118.80	510.0
123.90	104.0
127.80	386.0
128.80	205.0
129.80	386.0
130.80	172.0
134.80	192.0
136.80	142.0
139.80	104.0
140.90	1003.0
141.80	101.0
142.80	1004.0
144.90	137.0
145.80	144.0
147.80	232.0
149.80	107.0
154.80	319.0
156.90	166.0
160.80	103.0
171.90	347.0
173.00	664.0
173.90	86016.0
174.90	6436.0
175.90	81832.0
176.90	5228.0
177.80	242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.90	982.0
37.00	5640.0
37.90	5096.0
38.90	2107.0
39.80	206.0
43.90	1164.0
44.90	1098.0
46.90	1503.0
47.90	626.0
48.90	5197.0
49.90	24480.0
51.00	7656.0
51.90	366.0
54.90	352.0
55.90	1758.0
56.90	3324.0
57.90	186.0
59.90	1217.0
60.90	5698.0
62.00	6051.0
62.90	4451.0
64.00	493.0
64.90	304.0
66.90	345.0
67.90	12569.0
69.00	13519.0
69.90	974.0
72.00	720.0
72.90	5611.0
74.00	21624.0
75.00	66080.0
75.90	5770.0
76.90	927.0
77.90	561.0
78.80	3186.0
79.90	1094.0
80.90	3573.0
81.90	693.0
85.90	133.0
86.90	5501.0
87.90	5476.0
90.80	475.0
91.90	3315.0
92.90	5577.0
94.00	14400.0
95.00	131776.0
96.00	8793.0
96.90	292.0
103.80	566.0
104.70	180.0
105.80	507.0
106.80	116.0
114.80	134.0
115.80	465.0
116.80	655.0
117.80	413.0
118.80	566.0
124.00	127.0
127.80	442.0
128.80	251.0
129.80	421.0
130.80	179.0
134.80	226.0
136.80	138.0
140.90	1119.0
141.80	103.0
142.80	1107.0
144.90	160.0
145.90	123.0
147.80	243.0
149.80	135.0
154.80	283.0
156.90	176.0
158.80	113.0
160.80	130.0
171.80	352.0
173.00	664.0
173.90	95984.0
174.90	7229.0
175.90	91504.0
176.90	5801.0
177.80	243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.90	994.0
37.00	5408.0
37.90	4974.0
38.90	1989.0
39.80	202.0
43.90	1120.0
45.00	1028.0
46.90	1471.0
47.90	610.0
48.90	5290.0
50.00	23872.0
50.90	7358.0
51.90	362.0
54.90	346.0
55.90	1769.0
56.90	3195.0
57.90	155.0
59.90	1205.0
60.90	5624.0
62.00	5895.0
62.90	4267.0
64.00	505.0
64.90	256.0
66.90	358.0
67.90	12310.0
69.00	13377.0
69.90	947.0
72.00	658.0
72.90	5693.0
74.00	21448.0
75.00	64984.0
76.00	5612.0
76.90	836.0
77.90	574.0
78.90	3176.0
79.90	1070.0
80.90	3555.0
81.90	693.0
85.80	140.0
86.90	5445.0
87.90	5542.0
90.80	498.0
91.90	3369.0
92.90	5461.0
94.00	14278.0
95.00	130896.0
96.00	8506.0
96.90	266.0
103.80	537.0
104.70	166.0
105.80	527.0
112.70	103.0
114.80	133.0
115.80	430.0
116.90	633.0
117.80	402.0
118.80	586.0
124.00	116.0
127.80	472.0
128.80	244.0
129.80	389.0
130.80	167.0
134.80	225.0
136.80	148.0
140.90	1135.0
141.80	101.0
142.80	1113.0
144.80	156.0
145.90	110.0
147.90	216.0
149.80	136.0
154.80	241.0
156.80	183.0
158.90	128.0
160.80	138.0
171.80	341.0
173.00	671.0
173.90	97672.0
174.90	7156.0
175.90	93504.0
176.90	5925.0
177.80	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003