




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060118.D
 Acq On : 23 Jul 2024 16:34
 Operator : MD/SY
 Sample : P3300-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GA4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 04:23:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 24 04:18:44 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
 Supervised By :Semsettin Yesilyurt 07/26/2024

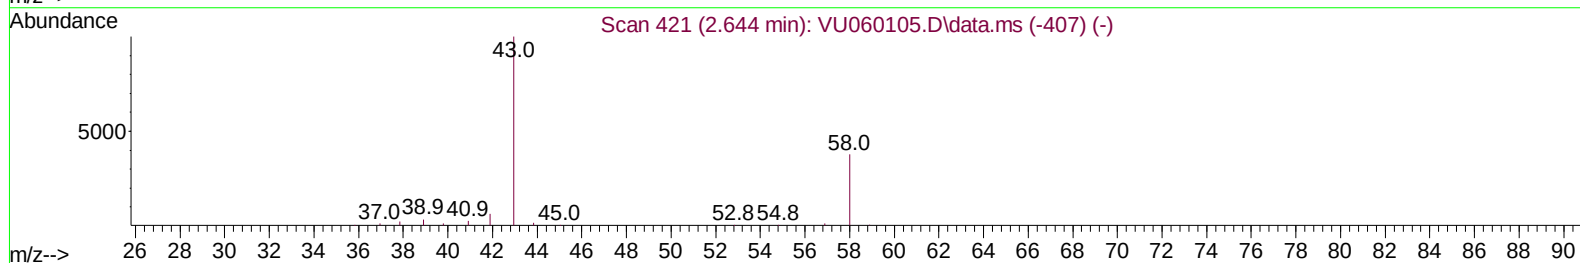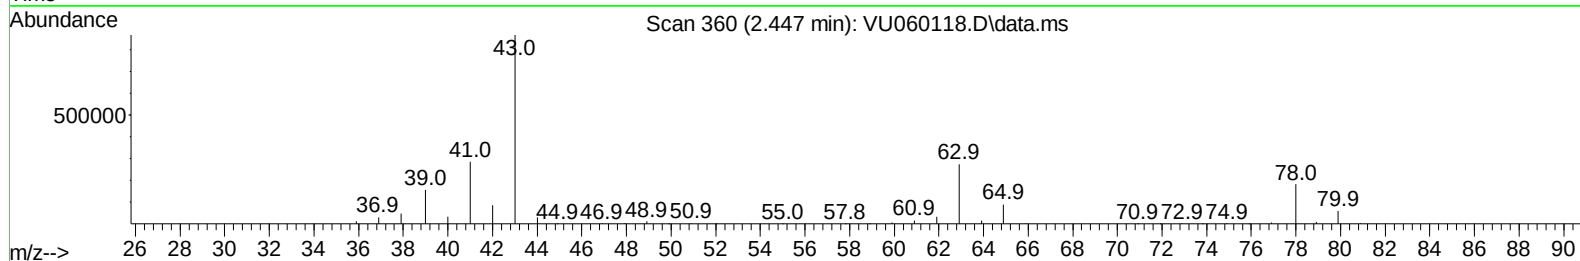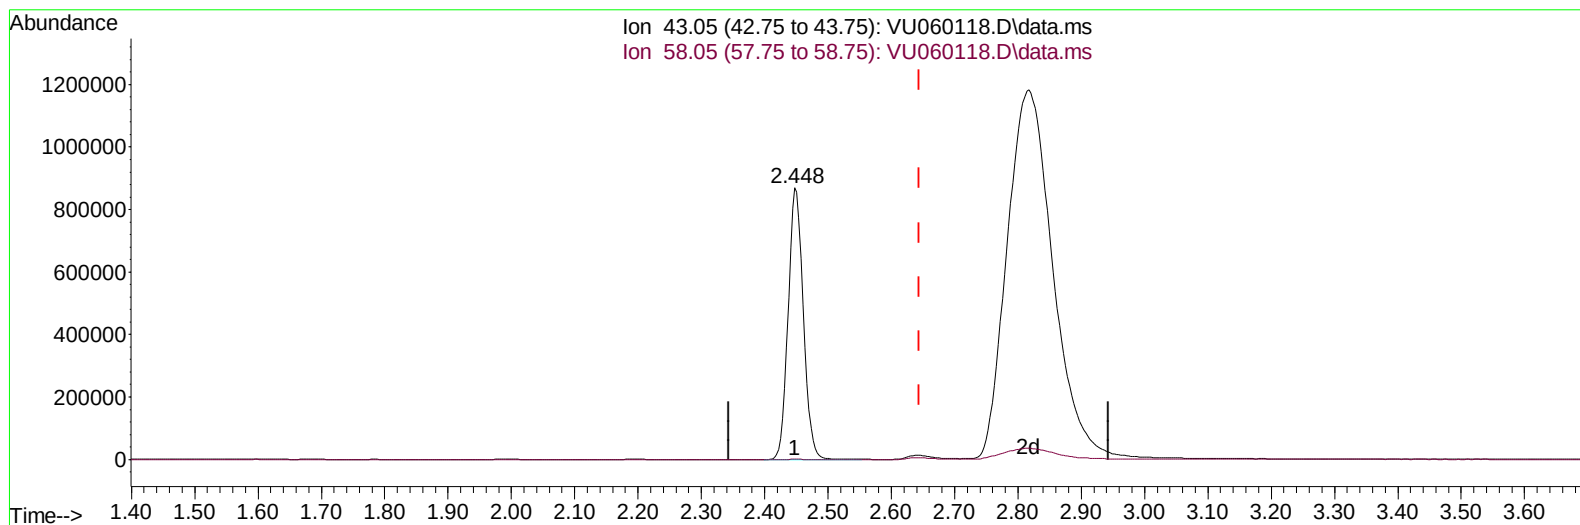

TIC: VU060118.D\data.ms

(13) Acetone (T)

2.447min (-0.196) 1177.83 ug/L

response 1447503

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	1.07
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060118.D
Acq On : 23 Jul 2024 16:34
Operator : MD/SY
Sample : P3300-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GA4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 04:23:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 04:18:44 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

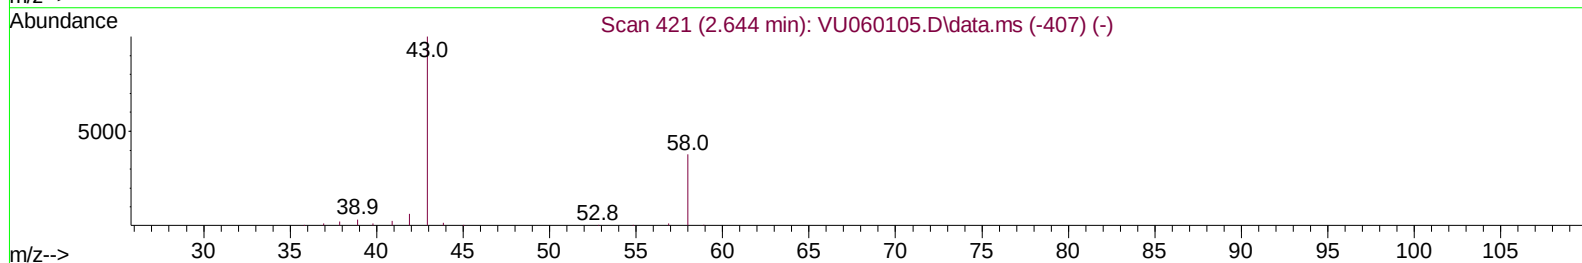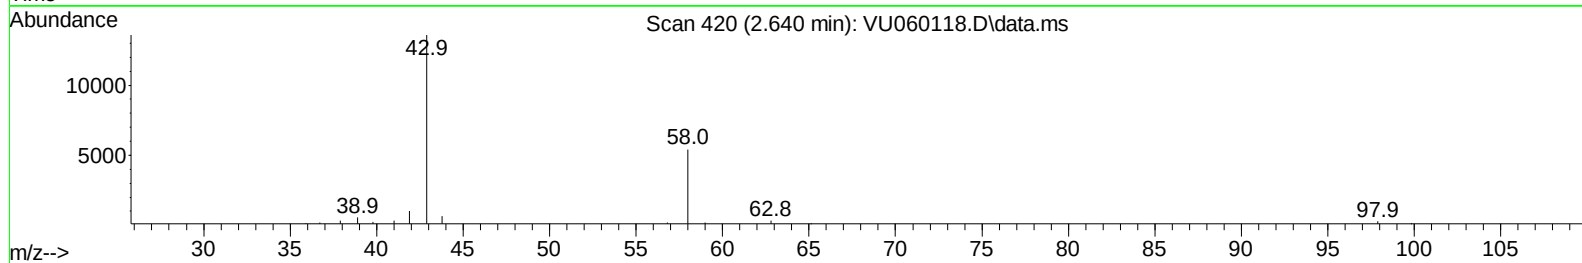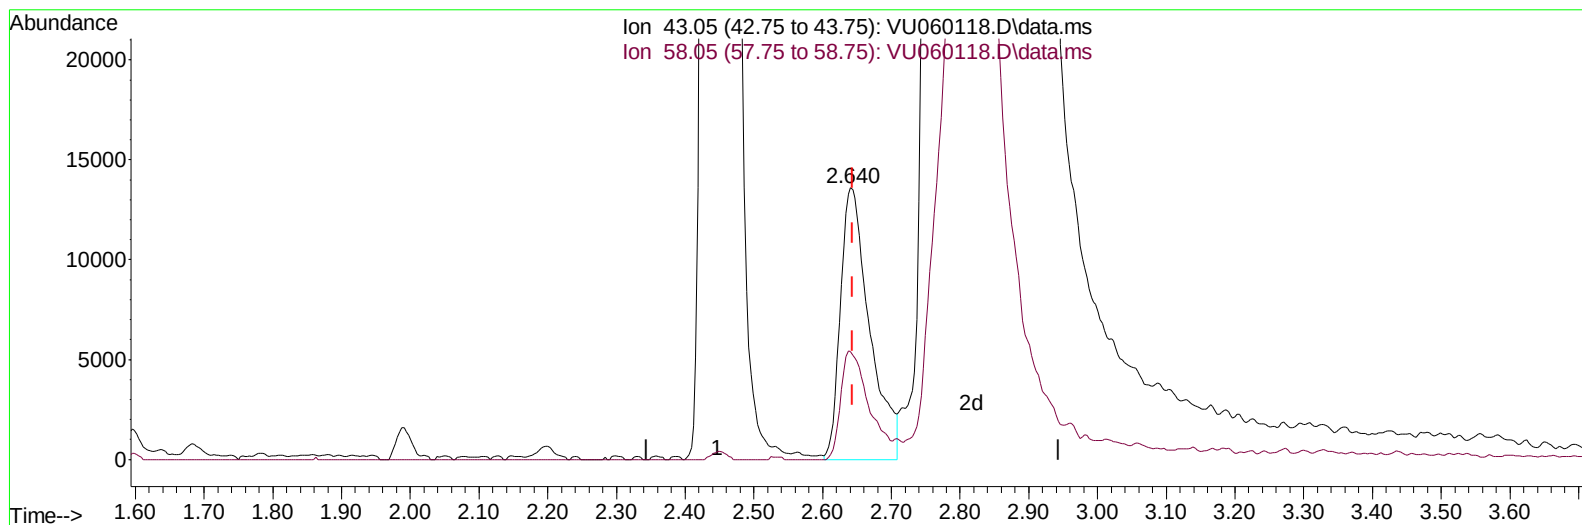

TIC: VU060118.D\data.ms

(13) Acetone (T)

2.640min (-0.003) 32.60 ug/L m

response 40065

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	38.76
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060118.D
 Acq On : 23 Jul 2024 16:34
 Operator : MD/SY
 Sample : P3300-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GA4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 04:23:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 24 04:18:44 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
 Supervised By :Semsettin Yesilyurt 07/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		114212	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117		120883	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		49787	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		31767	3.998	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%	
7) Chloroethane-d5	1.907	69		32448	4.395	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%	
11) 1,1-Dichloroethene-d2	2.560	65		12187	3.928	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.600%	
20) 2-Butanone-d5	4.627	46		94468	50.848	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.700%	
24) Chloroform-d	5.055	84		75561	4.524	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%	
26) 1,2-Dichloroethane-d4	5.695	65		38890	5.001	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.000%	
32) Benzene-d6	5.721	84		145686	4.498	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%	
36) 1,2-Dichloropropane-d6	6.685	67		49076	4.755	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.200%	
41) Toluene-d8	7.894	98		111713	3.818	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.400%	
43) trans-1,3-Dichloroprop...	8.180	79		8464	2.409	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	48.200%#	
46) 2-Hexanone-d5	8.627	63		58632	37.610	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.220%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		45367	4.939	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152		46157	5.136	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%	
Target Compounds							
13) Acetone	2.640	43		40065m	32.601	ug/L	
33) Benzene	5.772	78		5663	0.142	ug/L	100
42) Toluene	7.968	91		12464	0.293	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060118.D
Acq On : 23 Jul 2024 16:34
Operator : MD/SY
Sample : P3300-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GA4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

Quant Time: Jul 24 04:23:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 04:18:44 2024
Response via : Initial Calibration

