




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060136.D
Acq On : 24 Jul 2024 01:14
Operator : MD/SY
Sample : P3300-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB8

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

Quant Time: Jul 24 05:58:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 05:34:19 2024
Response via : Initial Calibration

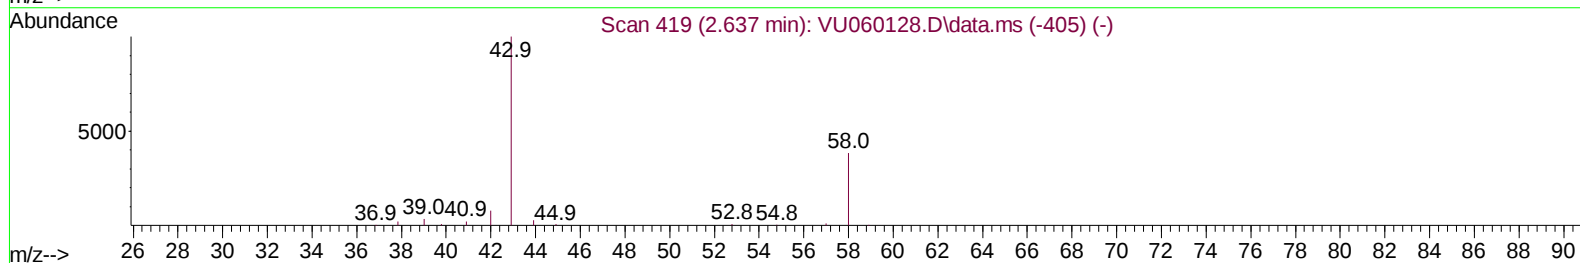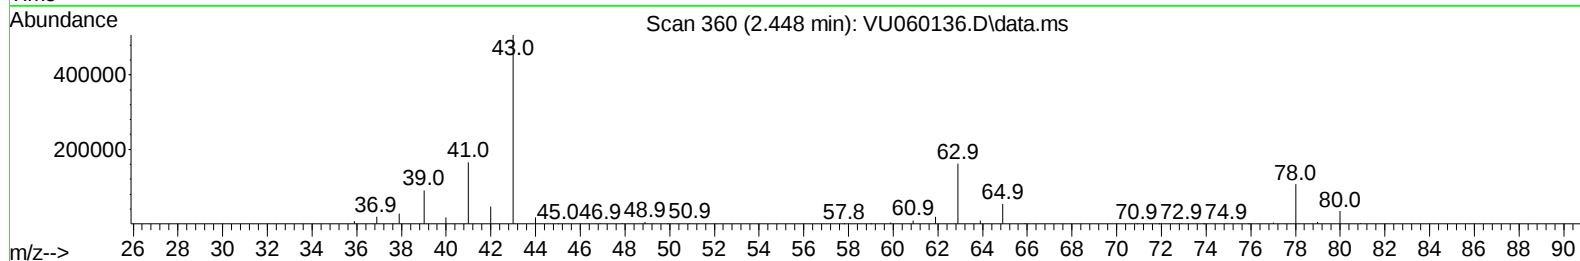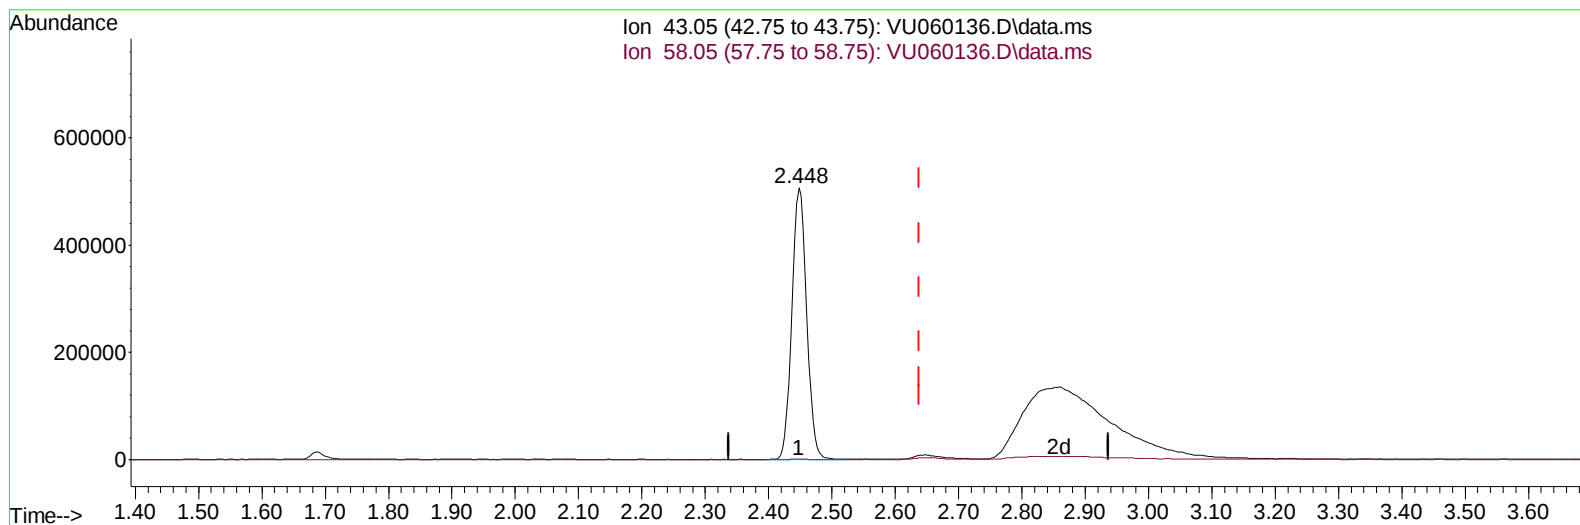

TIC: VU060136.D\data.ms

(13) Acetone (T)

2.448min (-0.190) 494.10 ug/L

response 822959

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	1.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060136.D
Acq On : 24 Jul 2024 01:14
Operator : MD/SY
Sample : P3300-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB8

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:58:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 05:34:19 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

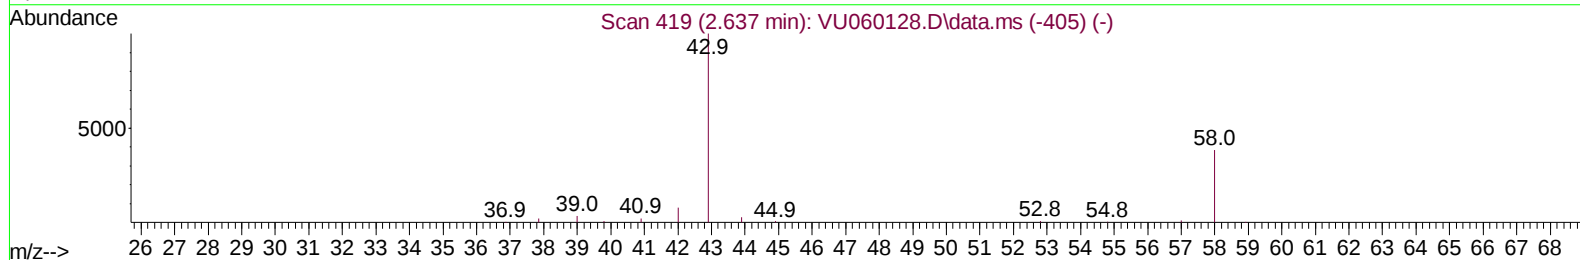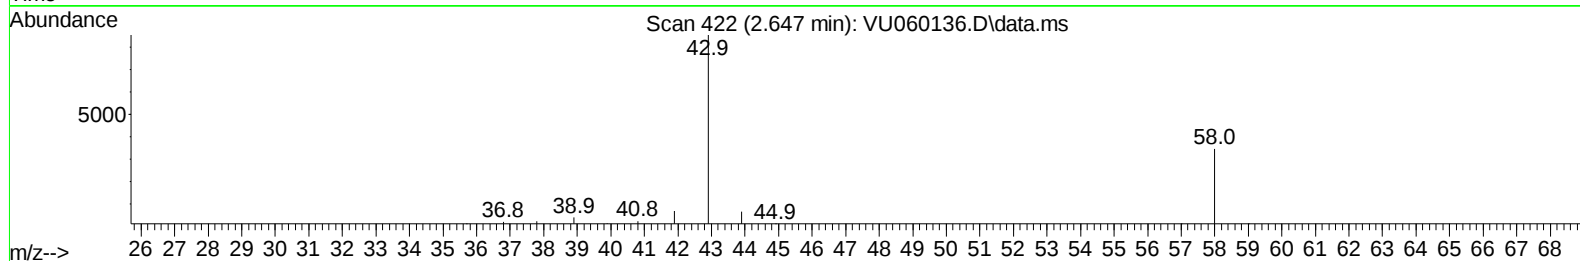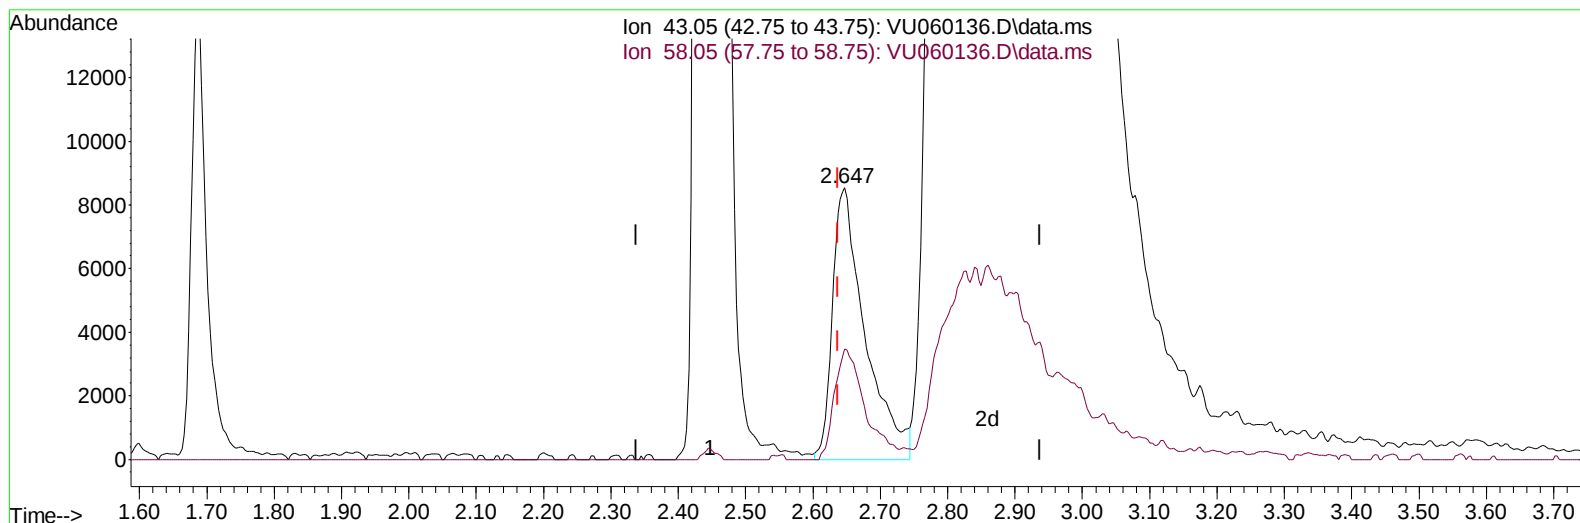

TIC: VU060136.D\data.ms

(13) Acetone (T)

2.647min (+ 0.010) 17.26 ug/L m

response 28745

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	38.06
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060136.D
 Acq On : 24 Jul 2024 01:14
 Operator : MD/SY
 Sample : P3300-22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GB8

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:58:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 24 05:34:19 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
 Supervised By :Semsettin Yesilyurt 07/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		154788	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		160919	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152		73478	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		51990	4.827	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	96.600%		
7) Chloroethane-d5	1.911	69		46067	4.604	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	92.000%		
11) 1,1-Dichloroethene-d2	2.560	65		20106	4.782	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	95.600%		
20) 2-Butanone-d5	4.631	46		111798	44.402	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	88.800%		
24) Chloroform-d	5.055	84		94594	4.179	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	83.600%		
26) 1,2-Dichloroethane-d4	5.695	65		45084	4.278	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	85.600%		
32) Benzene-d6	5.721	84		195592	4.537	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	90.800%		
36) 1,2-Dichloropropane-d6	6.682	67		61135	4.450	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	89.000%		
41) Toluene-d8	7.891	98		165900	4.259	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	85.200%		
43) trans-1,3-Dichloroprop...	8.177	79		18323	3.918	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	78.400%		
46) 2-Hexanone-d5	8.628	63		83980	40.468	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	80.940%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84		51973	4.251	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	85.000%		
66) 1,2-Dichlorobenzene-d4	12.187	152		66039	4.979	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	99.600%		
Target Compounds							Qvalue
13) Acetone	2.647	43		28745m	17.258	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060136.D
Acq On : 24 Jul 2024 01:14
Operator : MD/SY
Sample : P3300-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB8

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

Quant Time: Jul 24 05:58:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 05:34:19 2024
Response via : Initial Calibration

