




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060138.D
Acq On : 24 Jul 2024 02:02
Operator : MD/SY
Sample : P3300-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G96

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:59:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 05:34:19 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

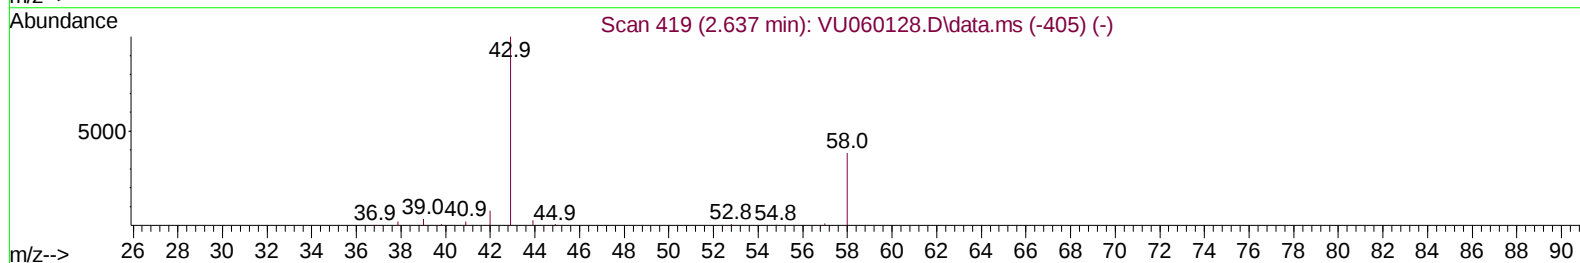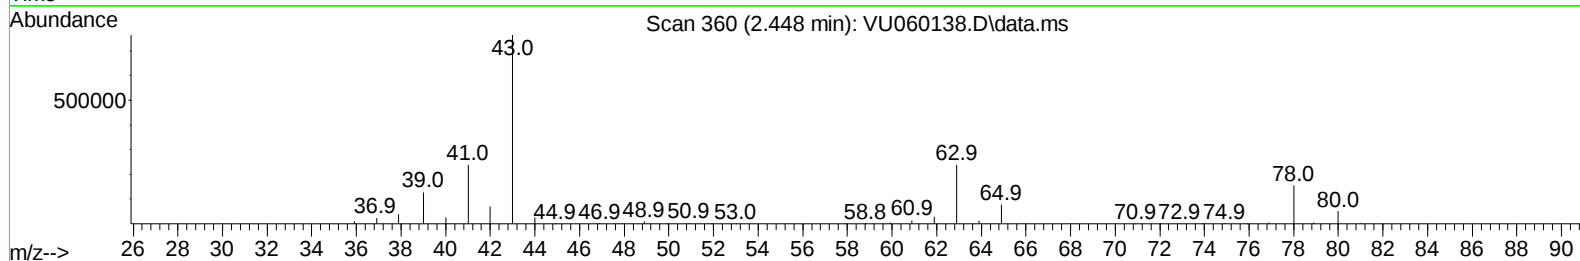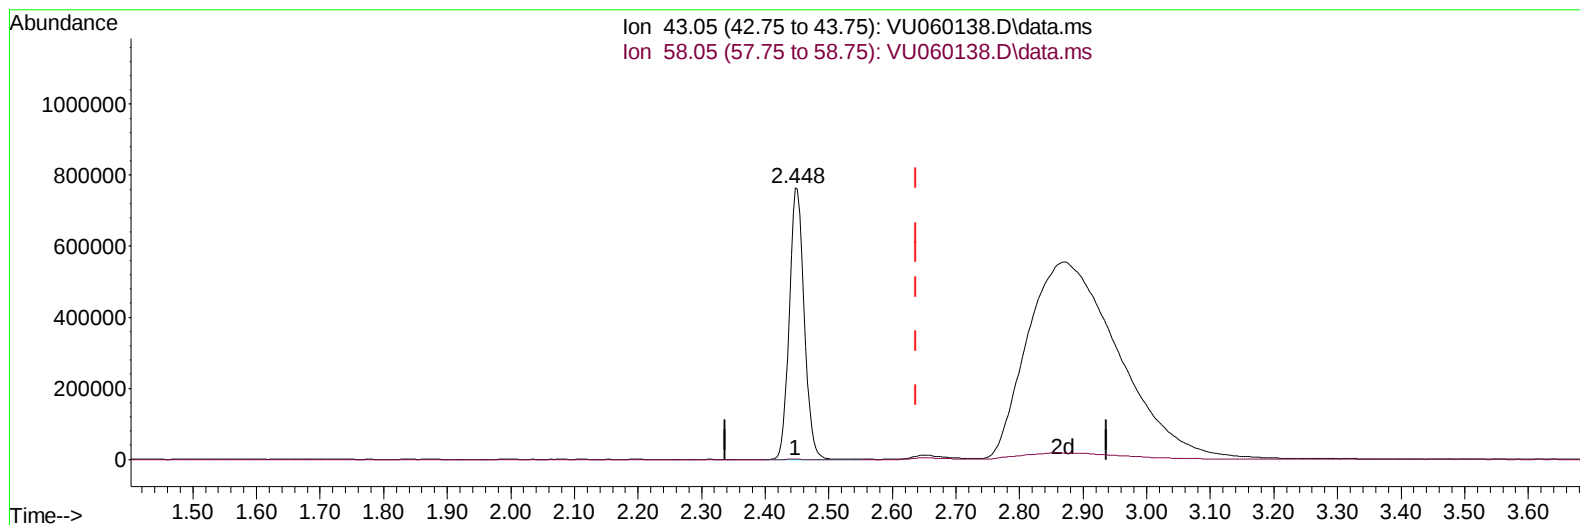

TIC: VU060138.D\data.ms

(13) Acetone (T)

2.448min (-0.190) 716.35 ug/L

response 1249195

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	1.42
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060138.D
Acq On : 24 Jul 2024 02:02
Operator : MD/SY
Sample : P3300-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G96

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:59:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 05:34:19 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

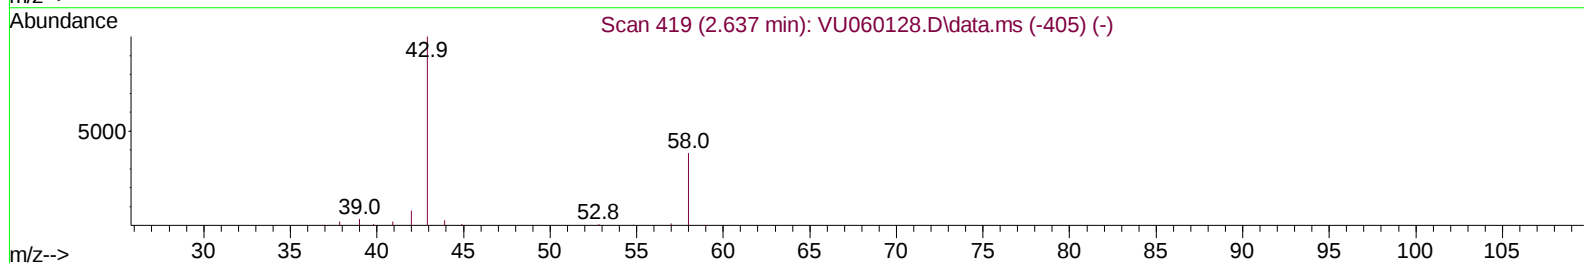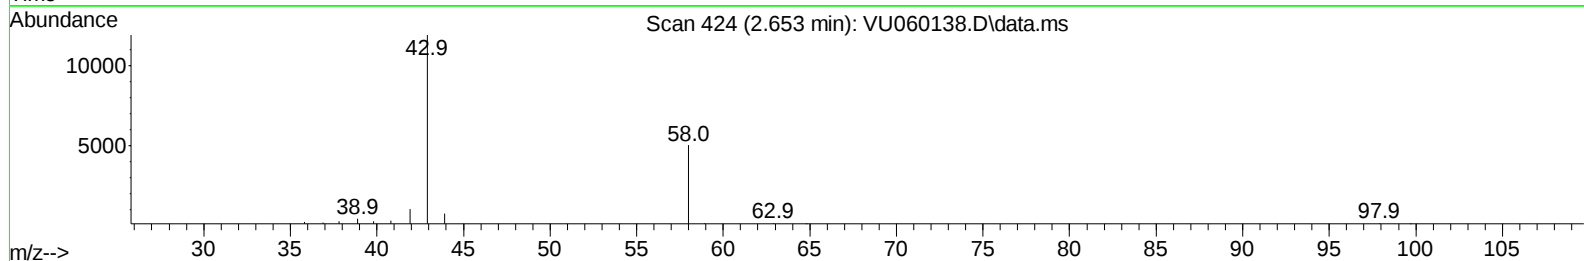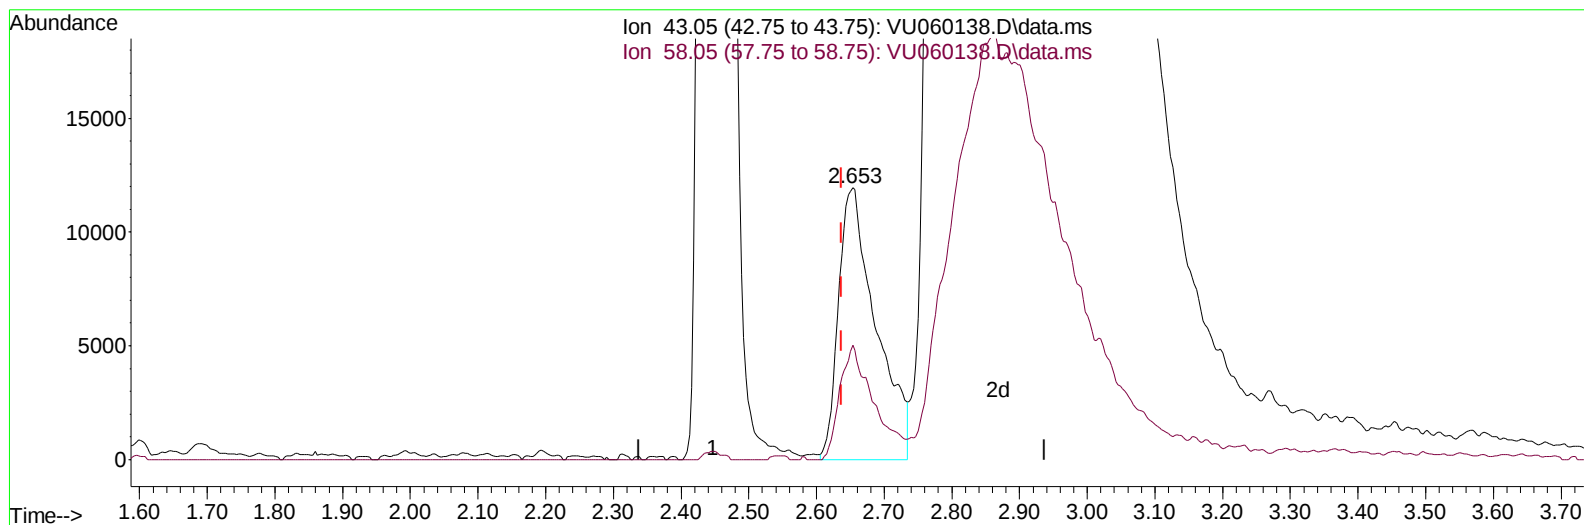

TIC: VU060138.D\data.ms

(13) Acetone (T)

2.653min (+ 0.016) 26.28 ug/L m

response 45827

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	38.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060138.D
 Acq On : 24 Jul 2024 02:02
 Operator : MD/SY
 Sample : P3300-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G96

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:59:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 24 05:34:19 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
 Supervised By :Semsettin Yesilyurt 07/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		162061	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		168227	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		77295	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		47831	4.242	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	84.800%		
7) Chloroethane-d5	1.911	69		42970	4.102	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	82.000%		
11) 1,1-Dichloroethene-d2	2.563	65		18262	4.148	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	83.000%		
20) 2-Butanone-d5	4.634	46		108869	41.298	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	82.600%		
24) Chloroform-d	5.055	84		88005	3.714	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	74.200%		
26) 1,2-Dichloroethane-d4	5.695	65		43642	3.955	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	79.200%		
32) Benzene-d6	5.721	84		183110	4.063	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	81.200%		
36) 1,2-Dichloropropane-d6	6.685	67		58818	4.095	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	82.000%		
41) Toluene-d8	7.894	98		154175	3.786	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	75.800%		
43) trans-1,3-Dichloroprop...	8.177	79		16907	3.458	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	69.200%		
46) 2-Hexanone-d5	8.627	63		84300	38.857	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	77.720%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84		49266	3.854	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	77.000%		
66) 1,2-Dichlorobenzene-d4	12.187	152		61326	4.396	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	88.000%		
Target Compounds							
13) Acetone	2.653	43		45827m	26.280	ug/L	
42) Toluene	7.965	91		26721	0.452	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060138.D
Acq On : 24 Jul 2024 02:02
Operator : MD/SY
Sample : P3300-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G96

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

Quant Time: Jul 24 05:59:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 05:34:19 2024
Response via : Initial Calibration

