




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060141.D
 Acq On : 24 Jul 2024 03:13
 Operator : MD/SY
 Sample : P3300-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:59:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 24 05:34:19 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
 Supervised By :Semsettin Yesilyurt 07/26/2024

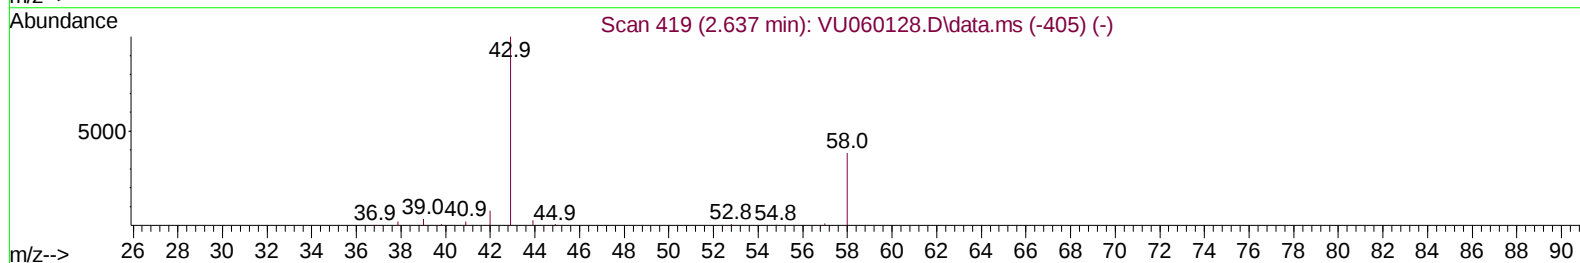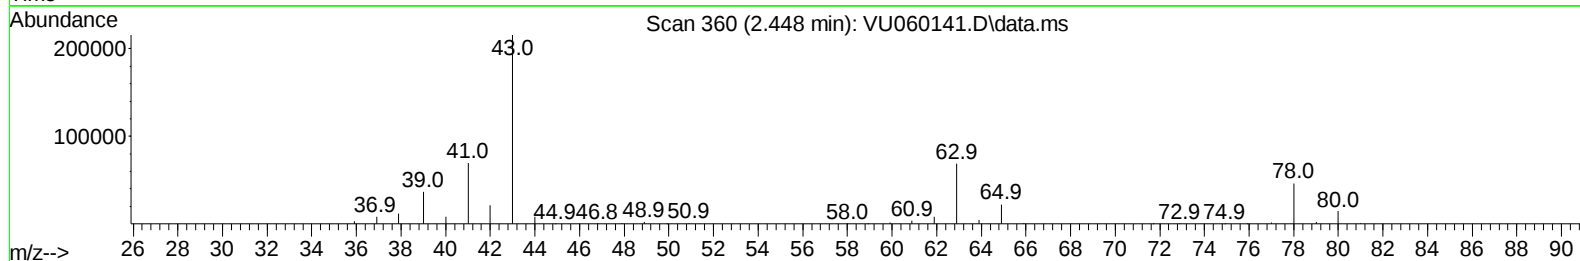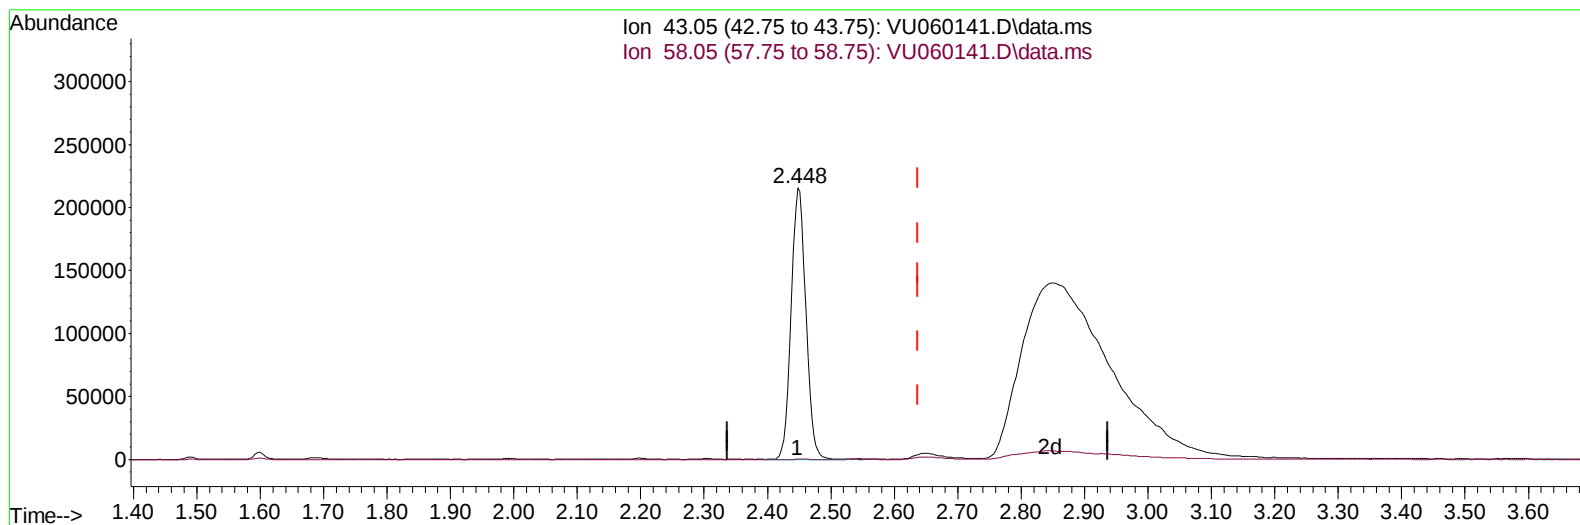

TIC: VU060141.D\data.ms

(13) Acetone (T)

2.448min (-0.190) 202.75 ug/L

response 347743

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	0.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060141.D
Acq On : 24 Jul 2024 03:13
Operator : MD/SY
Sample : P3300-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:59:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 05:34:19 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

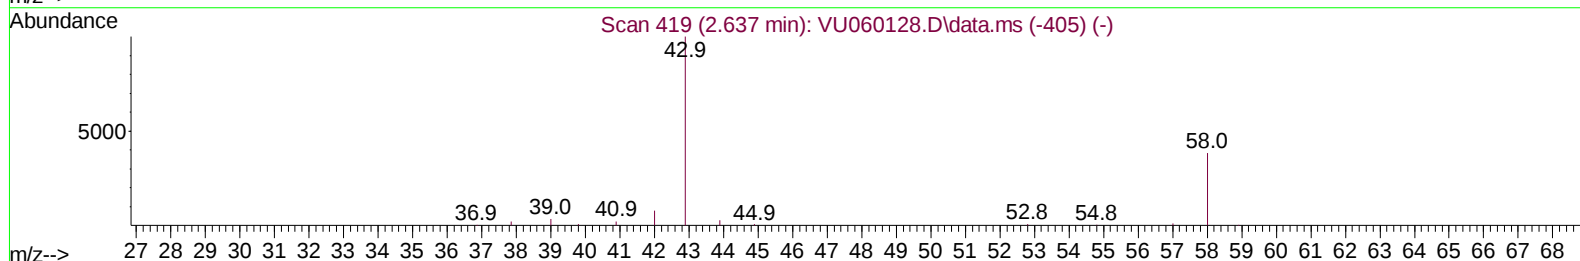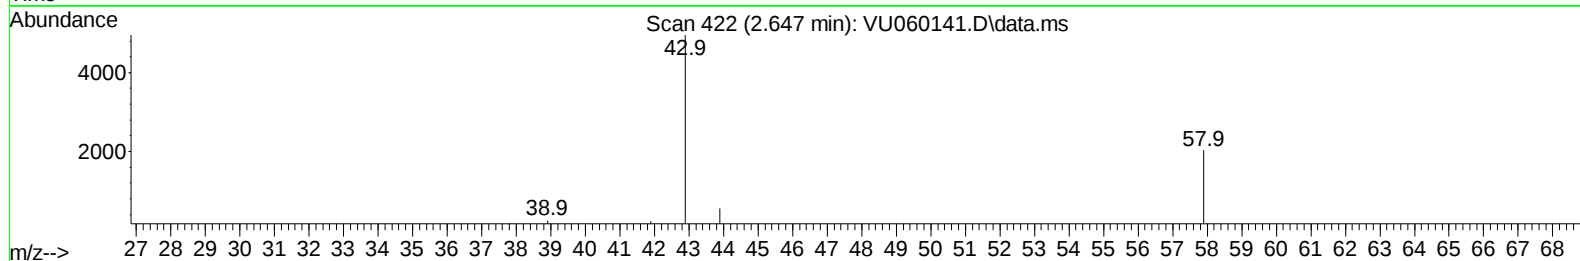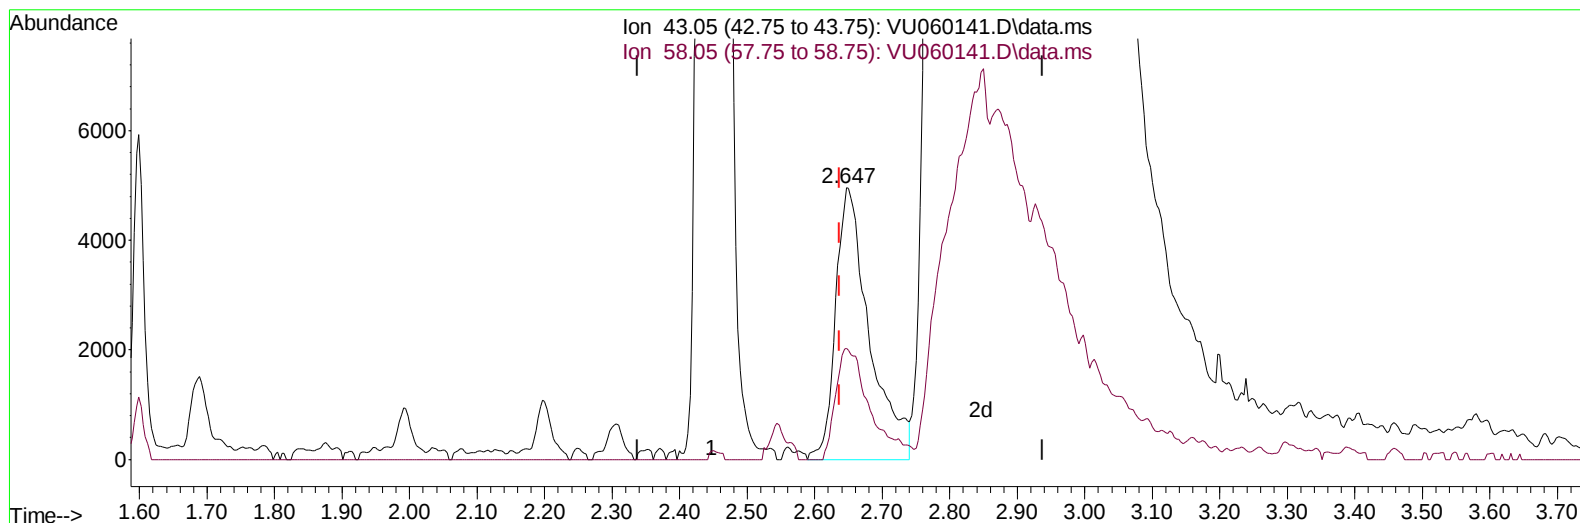

TIC: VU060141.D\data.ms

(13) Acetone (T)

2.647min (+ 0.010) 10.06 ug/L m

response 17254

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	6.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060141.D
 Acq On : 24 Jul 2024 03:13
 Operator : MD/SY
 Sample : P3300-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:59:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 24 05:34:19 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
 Supervised By :Semsettin Yesilyurt 07/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		159398	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		164839	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		70811	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		48557	4.378	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	87.600%	
7) Chloroethane-d5	1.911	69		43571	4.229	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	84.600%	
11) 1,1-Dichloroethene-d2	2.560	65		19313	4.460	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	89.200%	
20) 2-Butanone-d5	4.631	46		108749	41.942	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	83.880%	
24) Chloroform-d	5.055	84		90689	3.891	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	77.800%	
26) 1,2-Dichloroethane-d4	5.695	65		45614	4.203	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	84.000%	
32) Benzene-d6	5.721	84		182253	4.127	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	82.600%	
36) 1,2-Dichloropropane-d6	6.685	67		57163	4.062	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	81.200%	
41) Toluene-d8	7.891	98		153011	3.834	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	76.600%	
43) trans-1,3-Dichloroprop...	8.177	79		17745	3.704	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	74.000%	
46) 2-Hexanone-d5	8.627	63		80788	38.004	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	76.000%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		50511	4.033	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	80.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152		59922	4.688	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	93.800%	
Target Compounds							
5) vinyl chloride	1.602	62		6952	0.426	ug/L	84
13) Acetone	2.647	43		17254m	10.060	ug/L	
22) cis-1,2-Dichloroethene	4.657	96		79213	5.588	ug/L	98
25) Chloroform	5.081	83		7490	0.283	ug/L	96
34) Trichloroethene	6.538	95		20221	1.400	ug/L	99
42) Toluene	7.968	91		10782	0.186	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060141.D
Acq On : 24 Jul 2024 03:13
Operator : MD/SY
Sample : P3300-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 24 05:59:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 05:34:19 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/26/2024
Supervised By :Semsettin Yesilyurt 07/26/2024

