

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060114.D
 Acq On : 23 Jul 2024 14:58
 Operator : MD/SY
 Sample : P3325-02 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B29

Quant Time: Jul 24 04:22:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 24 04:18:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	148898	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	162486	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	69233	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	51102	4.933	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.600%
7) Chloroethane-d5	1.907	69	46056	4.785	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.800%
11) 1,1-Dichloroethene-d2	2.560	65	19800	4.895	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.000%
20) 2-Butanone-d5	4.624	46	97983	40.454	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.900%
24) Chloroform-d	5.055	84	91669	4.210	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.200%
26) 1,2-Dichloroethane-d4	5.698	65	45732	4.511	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.200%
32) Benzene-d6	5.721	84	187715	4.312	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
36) 1,2-Dichloropropane-d6	6.685	67	59783	4.310	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.200%
41) Toluene-d8	7.894	98	158556	4.031	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.600%
43) trans-1,3-Dichloroprop...	8.177	79	17911	3.793	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.800%
46) 2-Hexanone-d5	8.631	63	73869	35.252	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.500%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	49141	3.980	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	59315	4.746	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.000%
Target Compounds						
16) Methylene chloride	3.039	84	9335	0.670	ug/L	97
22) cis-1,2-Dichloroethene	4.666	96	1729	0.131	ug/L	85
34) Trichloroethene	6.537	95	61645	4.330	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060114.D
Acq On : 23 Jul 2024 14:58
Operator : MD/SY
Sample : P3325-02 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29

Quant Time: Jul 24 04:22:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 24 04:18:44 2024
Response via : Initial Calibration




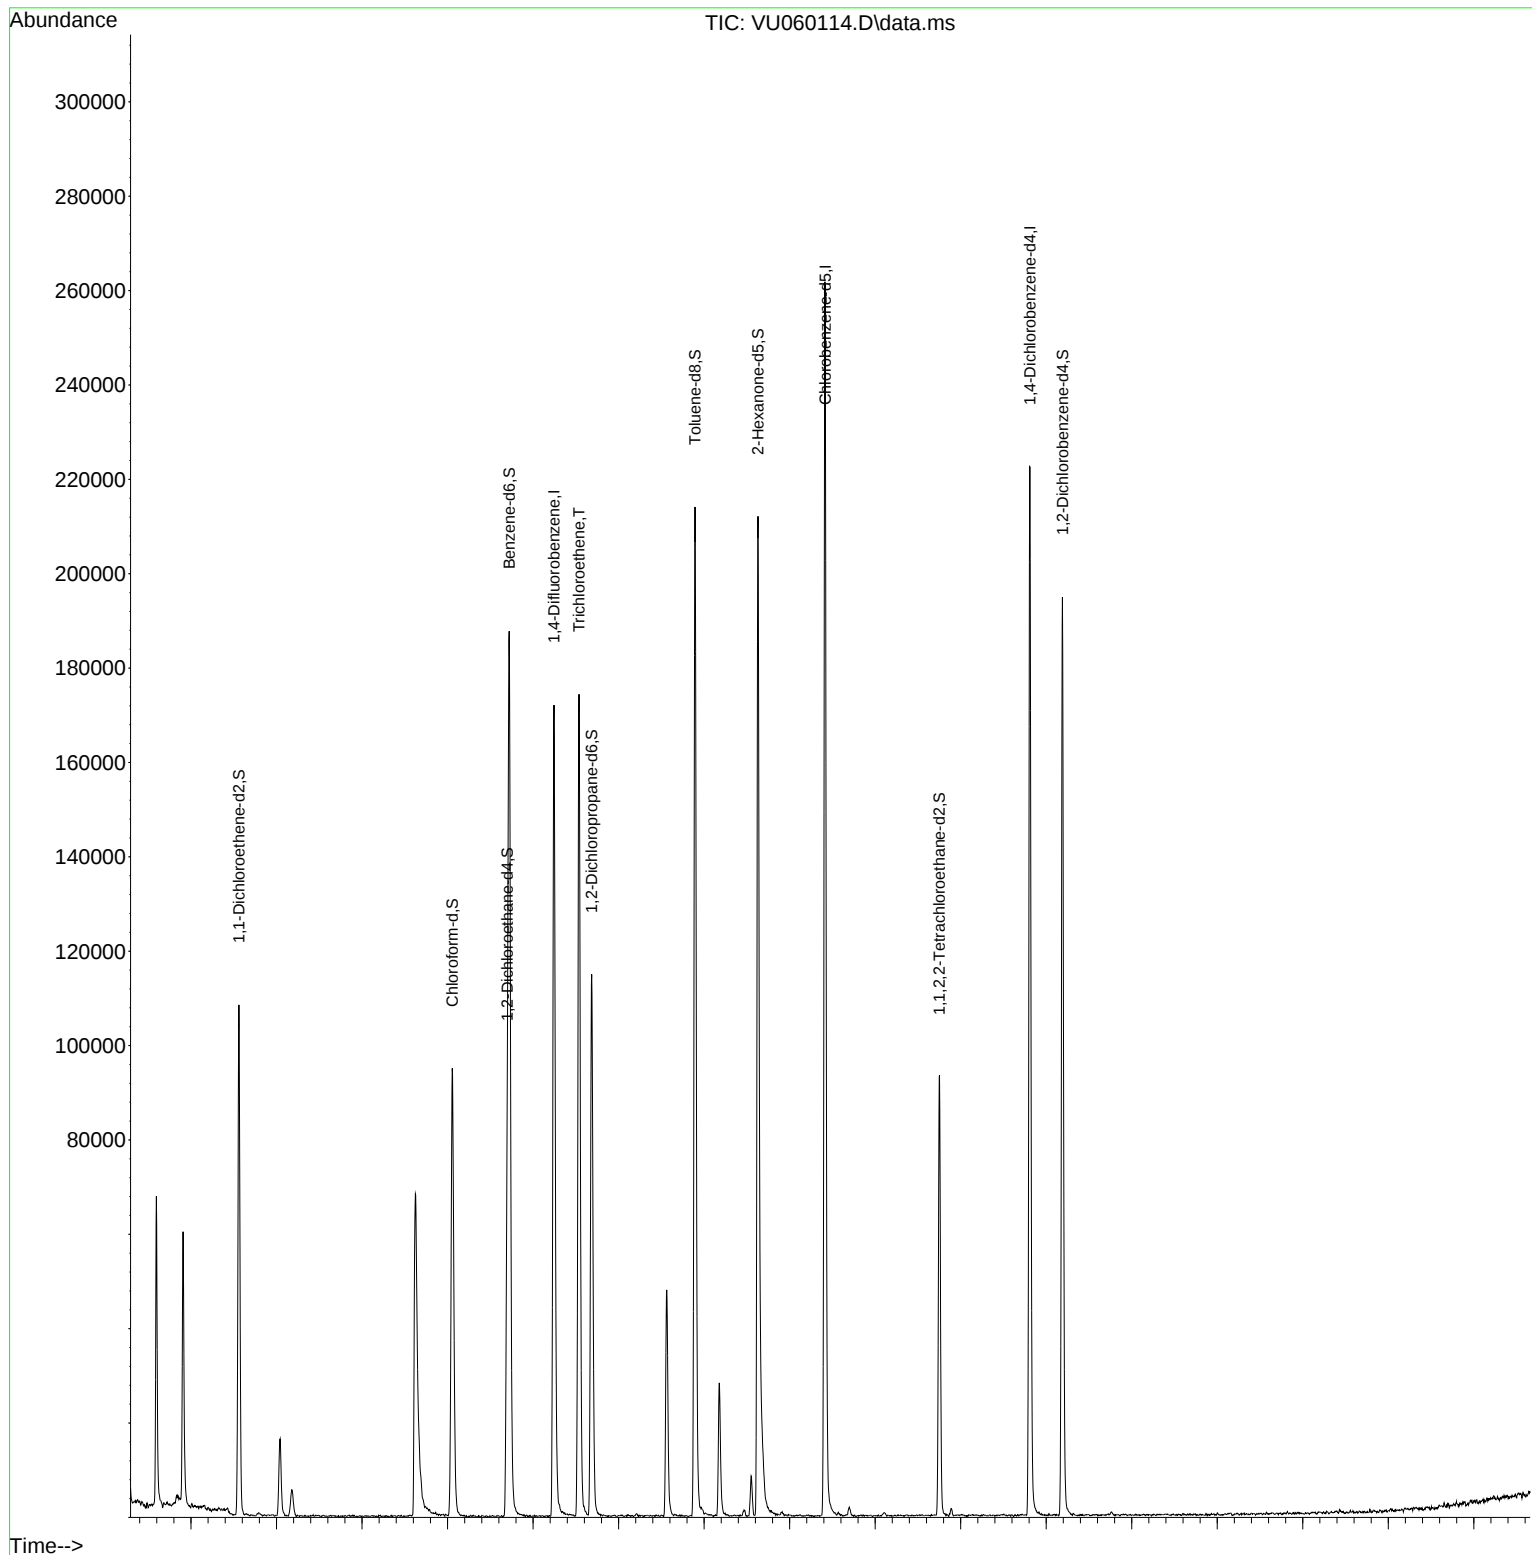


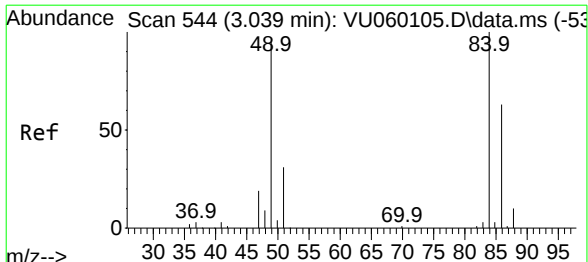

#16
Methylene chloride
Concen: 0.670 ug/L
RT: 3.039 min Scan# 54
Delta R.T. 0.000 min
Lab File: VU060114.D
Acq: 23 Jul 2024 14:58




Instrument :
MSVOA_U
ClientSampleId :
C0B29


Tgt Ion:	84	Resp:	9335
Ion	Ratio	Lower	Upper
84	100		
86	61.0	44.4	82.5
49	100.4	72.0	133.6

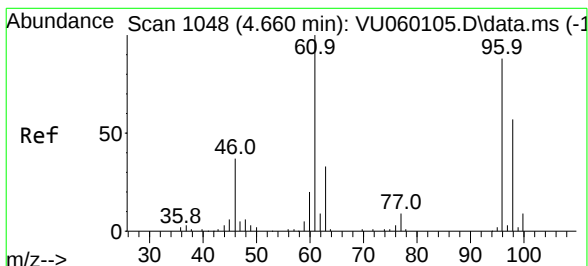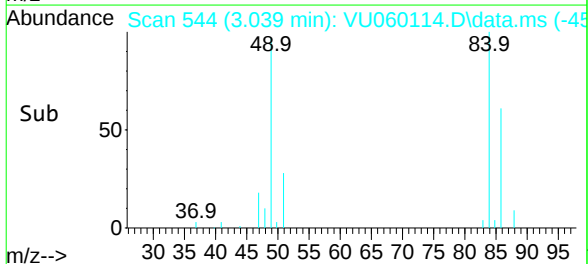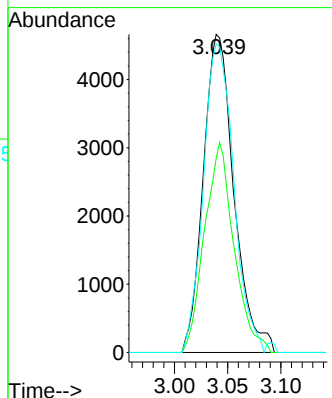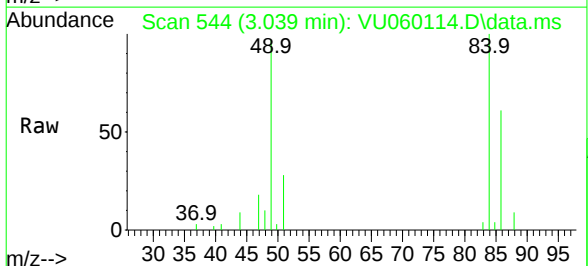

#22
cis-1,2-Dichloroethene
Concen: 0.131 ug/L
RT: 4.666 min Scan# 1050
Delta R.T. 0.006 min
Lab File: VU060114.D
Acq: 23 Jul 2024 14:58


Tgt Ion:	96	Resp:	1729
Ion	Ratio	Lower	Upper
96	100		
61	135.2	80.2	148.9
98	59.0	44.7	83.1

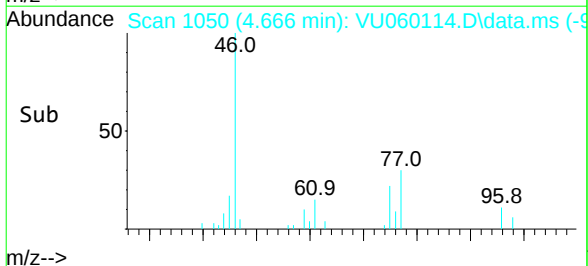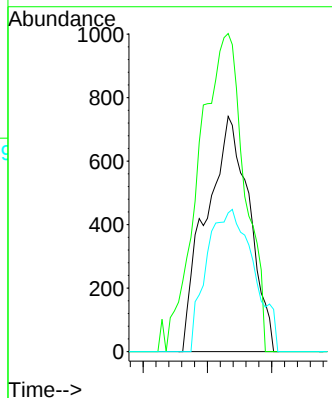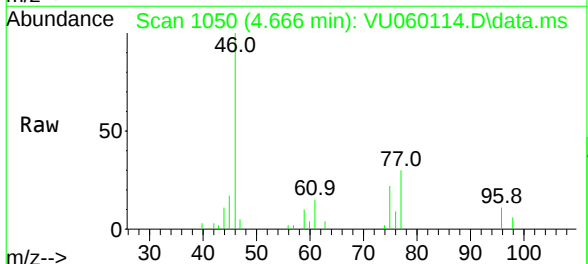

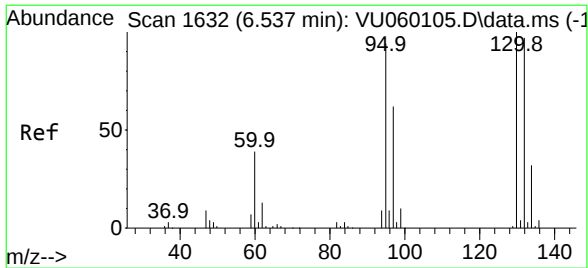

#34
 Trichloroethene
 Concen: 4.330 ug/L
 RT: 6.537 min Scan# 16
 Delta R.T. 0.000 min
 Lab File: VU060114.D
 Acq: 23 Jul 2024 14:58

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B29

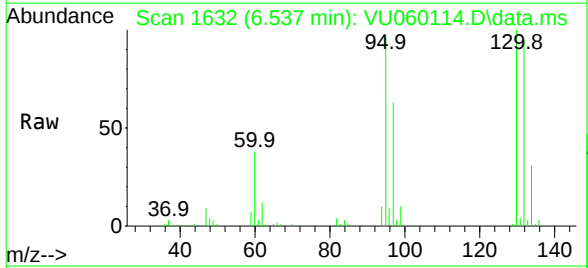

Tgt Ion:	95	Resp:	61645
Ion	Ratio	Lower	Upper
95	100		
97	65.6	45.9	85.3
132	98.1	71.4	132.6
130	103.7	72.1	133.9

