

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060111.D
 Acq On : 23 Jul 2024 13:45
 Operator : MD/SY
 Sample : P3325-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU060111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	85	95	109	rBV	67860	84180	17.55%	2.057%
2	1.908	183	192	210	rVB	54615	78347	16.33%	1.914%
3	2.560	383	395	409	rBV	103991	172822	36.03%	4.222%
4	3.039	533	544	562	rVB3	5734	11371	2.37%	0.278%
5	3.361	634	644	659	rVB8	2445	5145	1.07%	0.126%
6	4.621	1023	1036	1070	rBV	62292	166018	34.61%	4.056%
7	5.055	1156	1171	1194	rBV	92194	211446	44.08%	5.166%
8	5.721	1359	1378	1417	rBV2	183005	479633	100.00%	11.718%
9	6.245	1529	1541	1560	rBV	175845	340679	71.03%	8.323%
10	6.544	1623	1634	1646	rVB5	7205	13958	2.91%	0.341%
11	6.686	1666	1678	1694	rBV	110890	217447	45.34%	5.313%
12	7.563	1940	1951	1964	rBV2	46954	85540	17.83%	2.090%
13	7.894	2039	2054	2072	rBV	209687	369774	77.10%	9.034%
14	7.968	2074	2077	2092	rVB4	4685	7144	1.49%	0.175%
15	8.177	2129	2142	2159	rBV2	28129	50976	10.63%	1.245%
16	8.554	2249	2259	2267	rBV4	3660	5870	1.22%	0.143%
17	8.631	2271	2283	2320	rBV2	206582	418509	87.26%	10.225%
18	9.415	2512	2527	2557	rBV	264724	464221	96.79%	11.342%
19	9.570	2567	2575	2584	rBV3	3205	4871	1.02%	0.119%
20	9.698	2605	2615	2627	rVB2	3509	5841	1.22%	0.143%
21	10.110	2732	2743	2757	rBV6	3809	8521	1.78%	0.208%
22	10.483	2851	2859	2869	rBV3	3221	4995	1.04%	0.122%
23	10.753	2931	2943	2960	rBV	89991	152010	31.69%	3.714%
24	11.807	3260	3271	3294	rVV	233536	388095	80.91%	9.482%
25	12.190	3378	3390	3415	rBV	197728	333443	69.52%	8.147%
26	15.232	4327	4336	4344	rBV3	3111	5341	1.11%	0.130%
27	15.415	4385	4393	4407	rVB4	3582	6800	1.42%	0.166%




Sum of corrected areas: 4092997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060111.D
Acq On : 23 Jul 2024 13:45
Operator : MD/SY
Sample : P3325-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

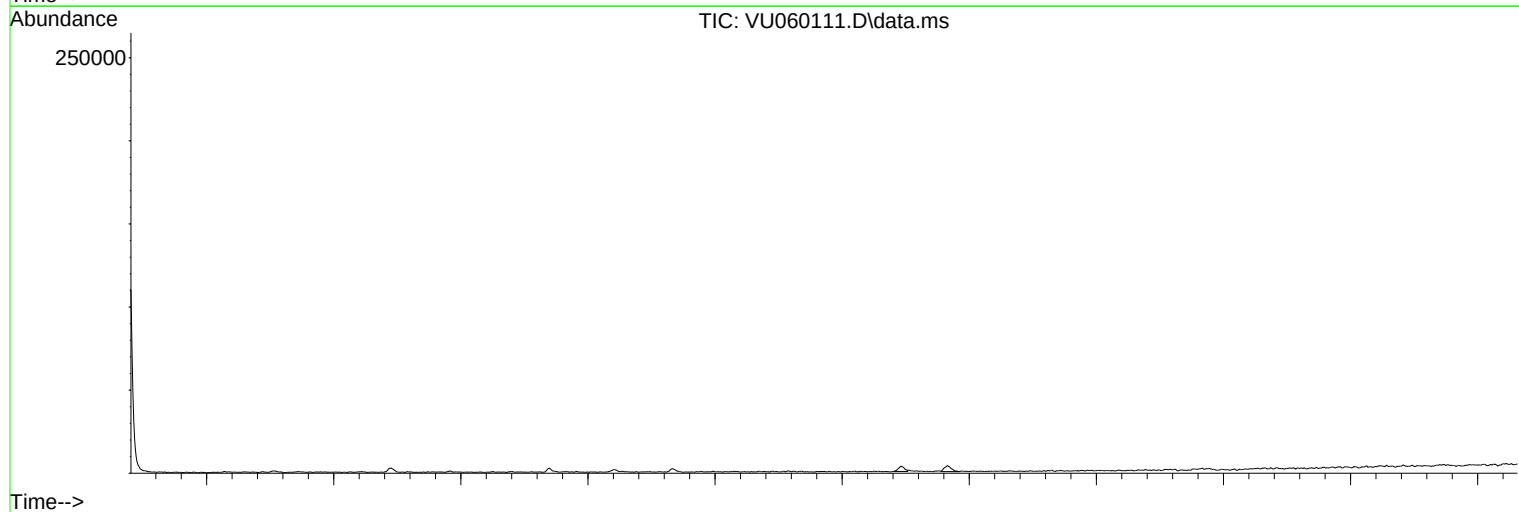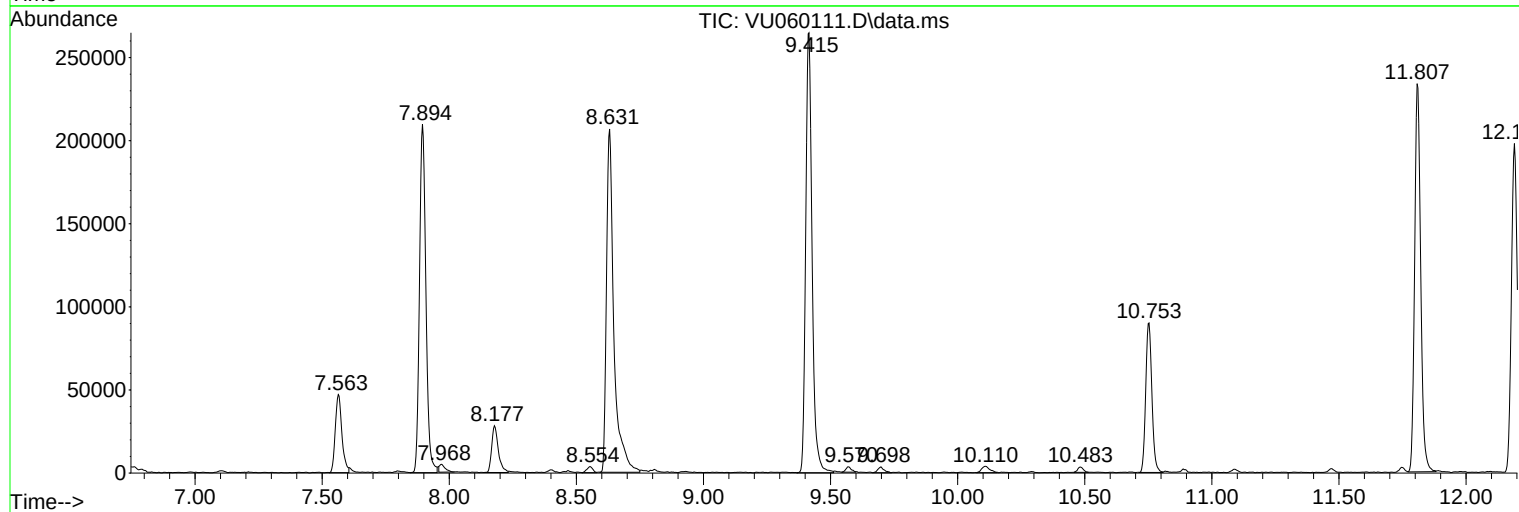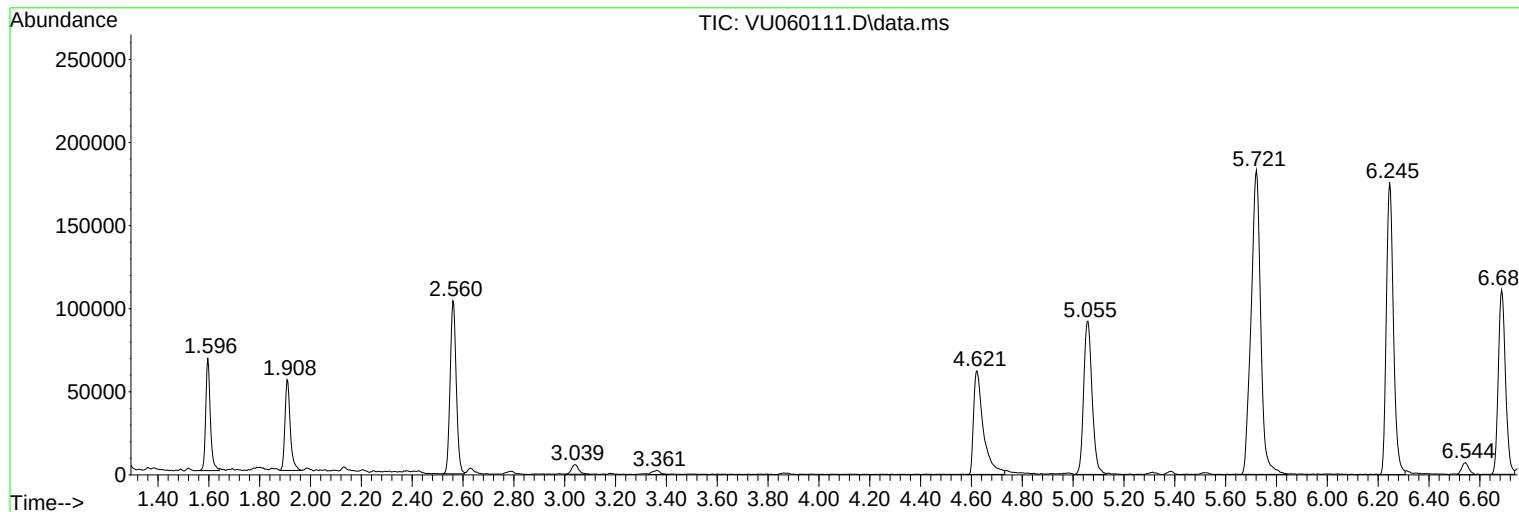

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060111.D
Acq On : 23 Jul 2024 13:45
Operator : MD/SY
Sample : P3325-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060111.D
Acq On : 23 Jul 2024 13:45
Operator : MD/SY
Sample : P3325-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------