

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060117.D
Acq On : 23 Jul 2024 16:10
Operator : MD/SY
Sample : P3300-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G91

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Title : TRACE VOA SFAM1.0

Signal : TIC: VU060117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.447	346	360	383	rVB	1111312	1839385	5.70%	5.058%
2	2.808	442	472	540	rBV	6780947	32295007	100.00%	88.812%
3	5.717	1359	1377	1406	rBV2	151834	407039	1.26%	1.119%
4	7.965	2065	2076	2108	rVB	596378	1038218	3.21%	2.855%
5	8.631	2270	2283	2314	rBV3	213180	451827	1.40%	1.243%
6	9.412	2508	2526	2555	rBV	188809	331681	1.03%	0.912%




Sum of corrected areas: 36363157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060117.D
Acq On : 23 Jul 2024 16:10
Operator : MD/SY
Sample : P3300-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

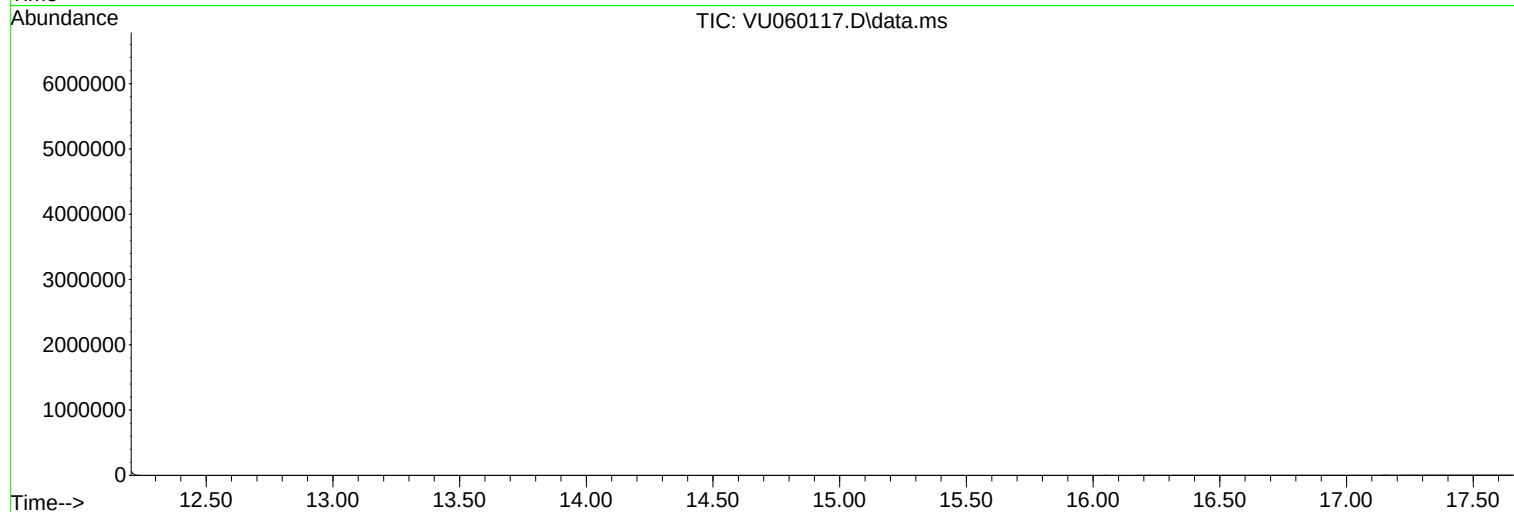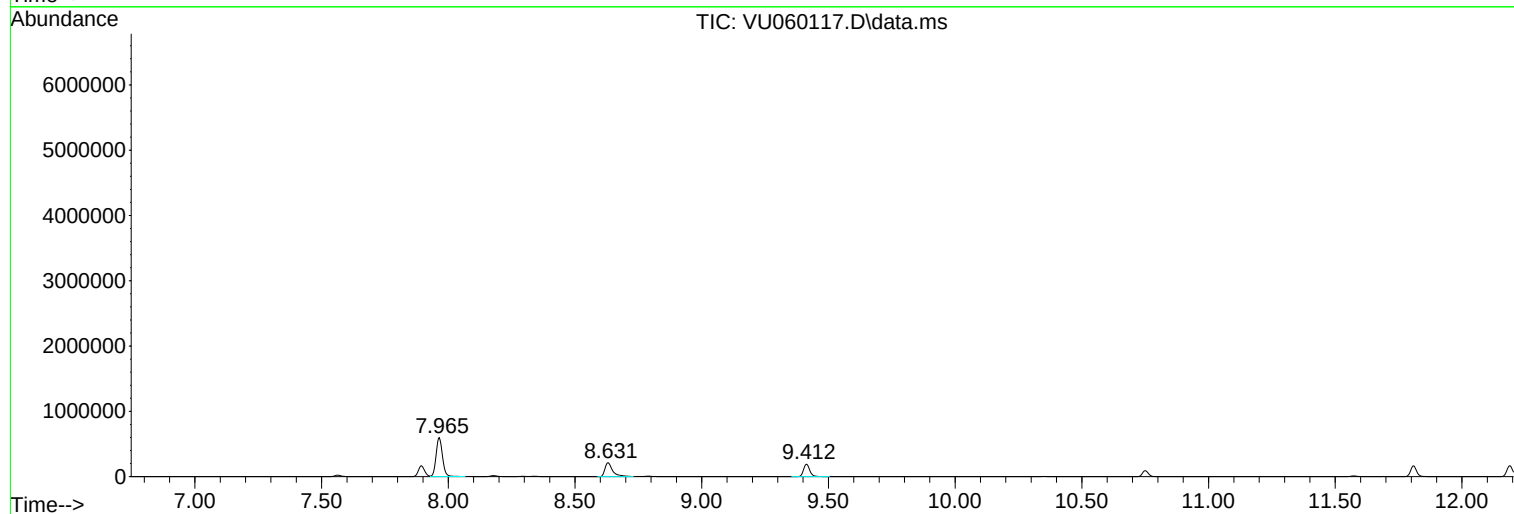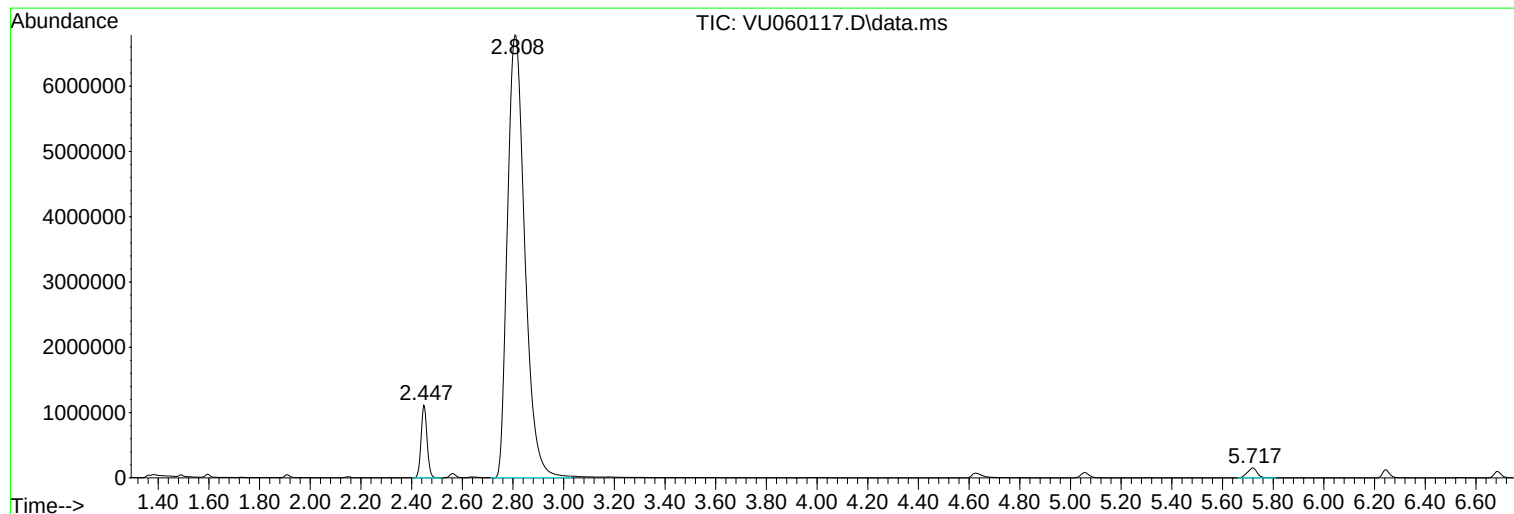

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060117.D
Acq On : 23 Jul 2024 16:10
Operator : MD/SY
Sample : P3300-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G91










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.447	22.59 ug/L	1839390	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	50
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	42
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

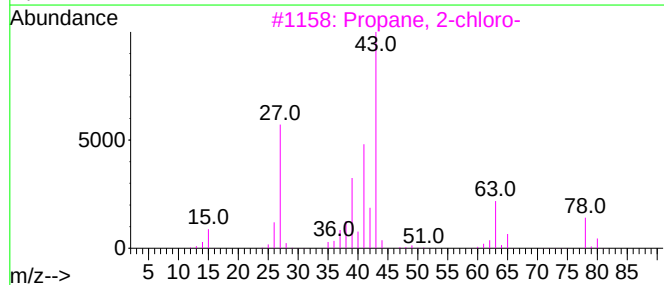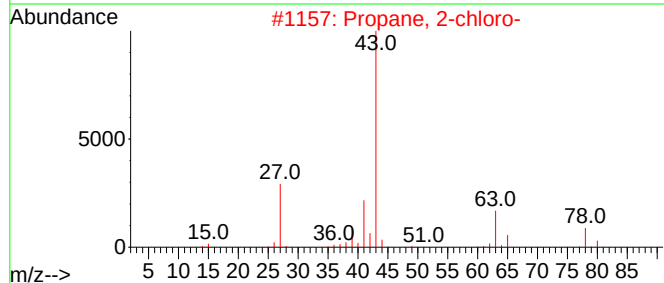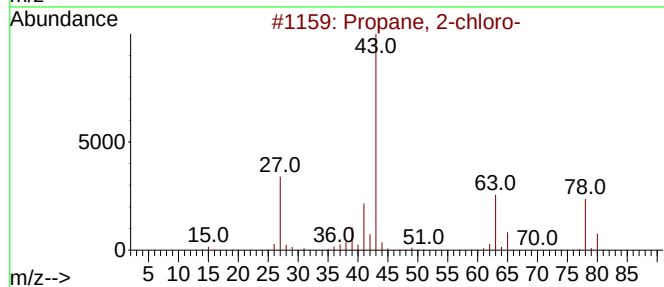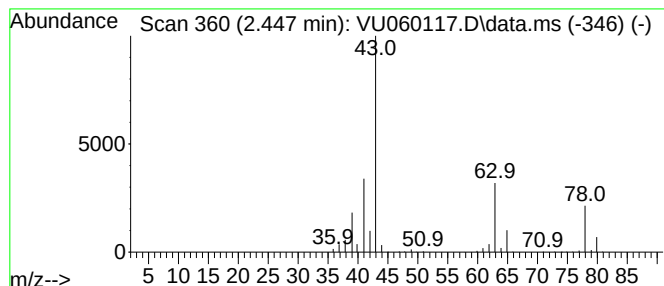

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060117.D
Acq On : 23 Jul 2024 16:10
Operator : MD/SY
Sample : P3300-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G91










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.808	396.71 ug/L	32295000	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
5			Propanoic acid, 2-hydroxy-, meth...	104	C4H8O3	000547-64-8	9

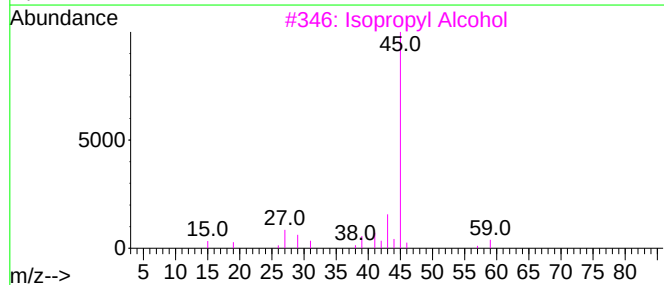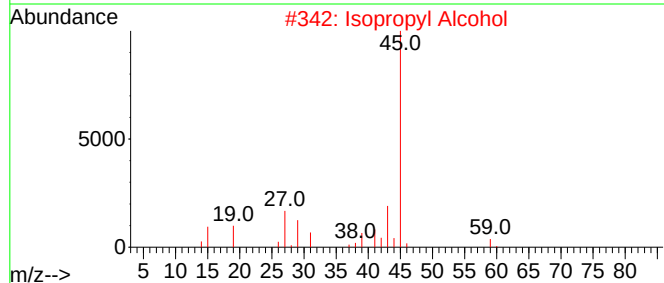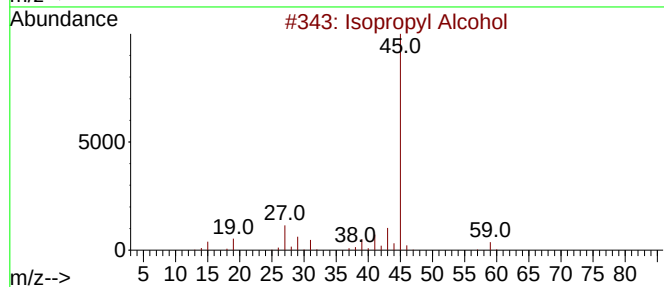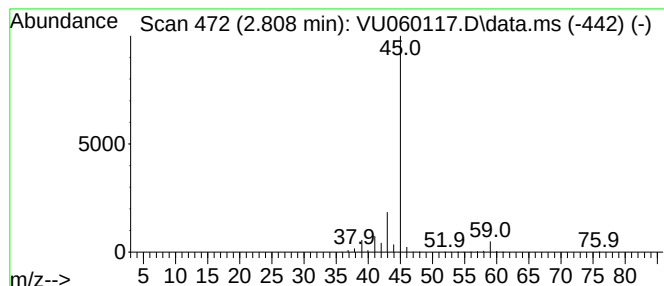

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060117.D
Acq On : 23 Jul 2024 16:10
Operator : MD/SY
Sample : P3300-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.447	22.6	ug/L	1839390	1	6.245	407039	5.0
Isopropyl Alcohol	2.808	396.7	ug/L	32295000	1	6.245	407039	5.0