

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060133.D
 Acq On : 24 Jul 2024 00:03
 Operator : MD/SY
 Sample : P3300-25
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GE8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.447	347	360	381	rVB	514868	838215	7.72%	5.310%
2	2.560	381	395	409	rBV	106089	173878	1.60%	1.101%
3	2.644	409	421	450	rBV	36806	117467	1.08%	0.744%
4	2.853	450	486	611	rVV2	1161632	10859594	100.00%	68.794%
5	4.631	1028	1039	1089	rBV	59554	211570	1.95%	1.340%
6	5.055	1154	1171	1194	rBV2	95461	215940	1.99%	1.368%
7	5.717	1355	1377	1403	rBV2	191246	491537	4.53%	3.114%
8	6.242	1528	1540	1568	rBV	187190	360287	3.32%	2.282%
9	6.685	1663	1678	1702	rBV	112590	224221	2.06%	1.420%
10	7.891	2041	2053	2067	rBV	220263	388785	3.58%	2.463%
11	8.630	2271	2283	2320	rBV2	228231	467391	4.30%	2.961%
12	9.412	2514	2526	2550	rBV	276102	473793	4.36%	3.001%
13	10.749	2931	2942	2962	rBV	95399	155868	1.44%	0.987%
14	11.807	3257	3271	3293	rBV	256524	434640	4.00%	2.753%
15	12.187	3377	3389	3410	rBV	215176	372451	3.43%	2.359%




Sum of corrected areas: 15785637

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060133.D
Acq On : 24 Jul 2024 00:03
Operator : MD/SY
Sample : P3300-25
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

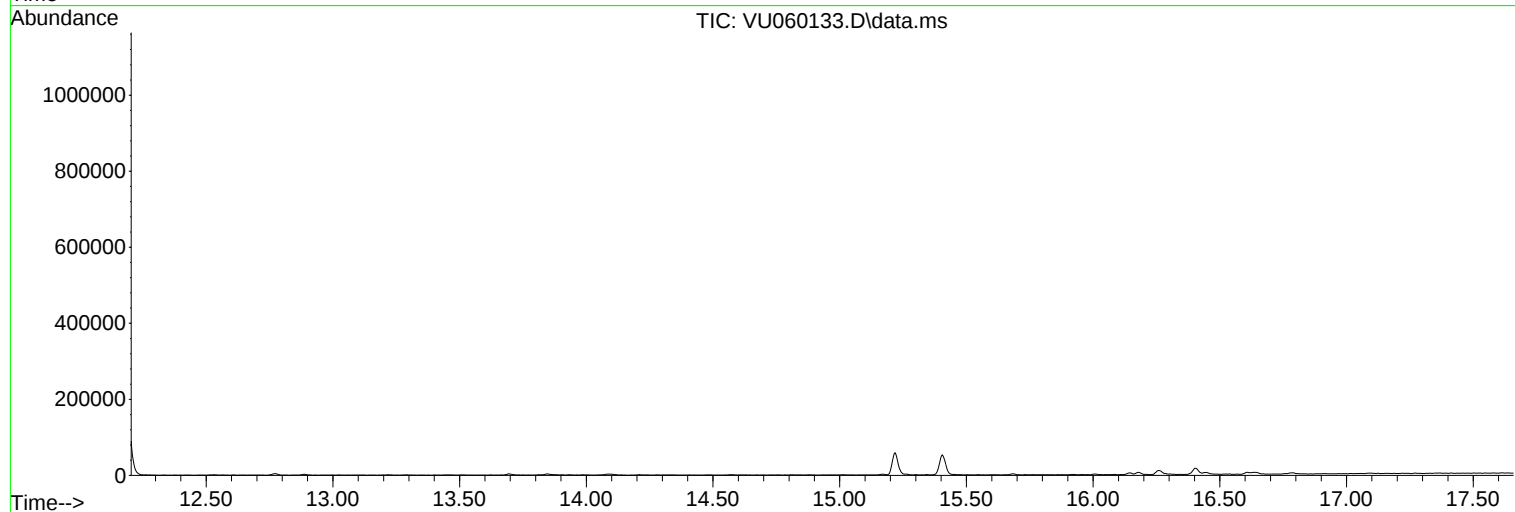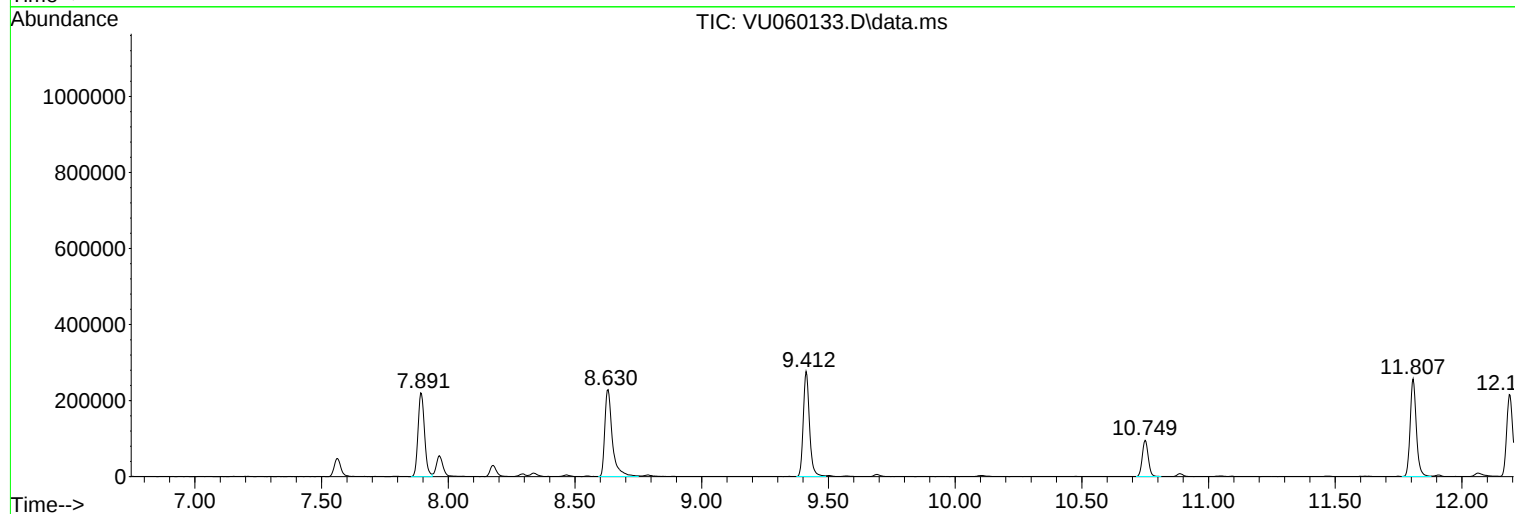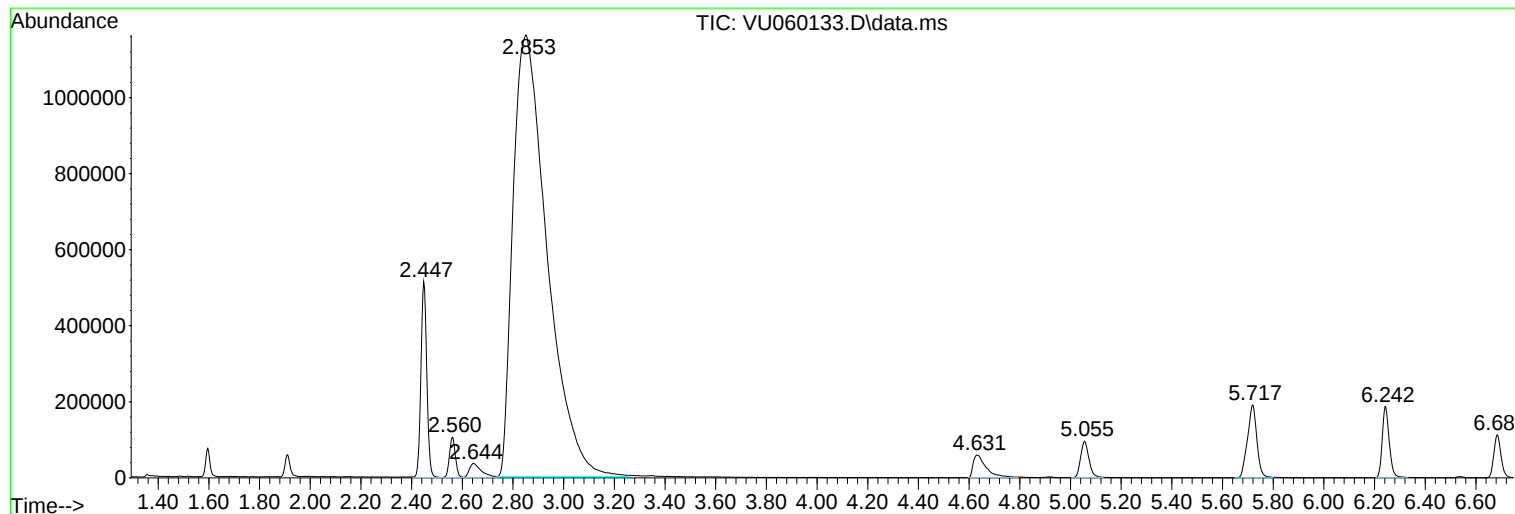

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060133.D
Acq On : 24 Jul 2024 00:03
Operator : MD/SY
Sample : P3300-25
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE8







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.447	11.63 ug/L	838215	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	78
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	42
4	Acetyl chloride			78	C2H3ClO	000075-36-5	9
5	2-Chloroethanol			80	C2H5ClO	000107-07-3	4

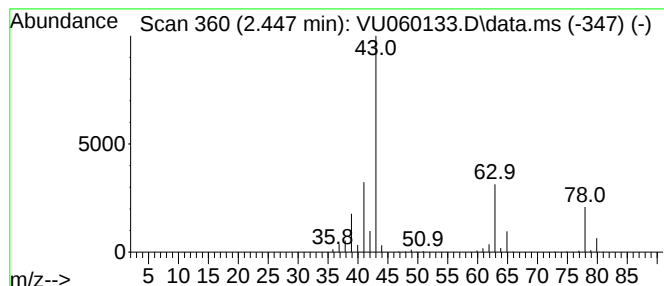

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060133.D
Acq On : 24 Jul 2024 00:03
Operator : MD/SY
Sample : P3300-25
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.853	150.71 ug/L	10859600	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	56
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

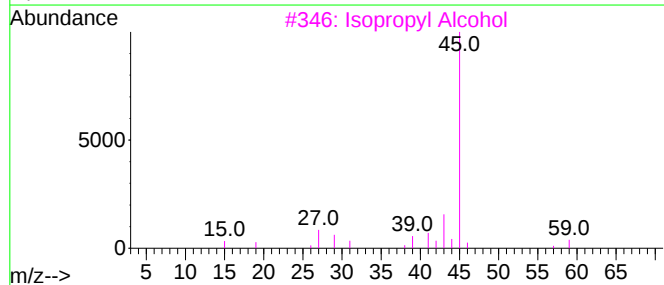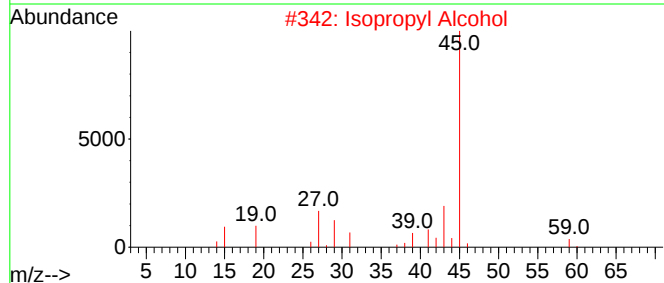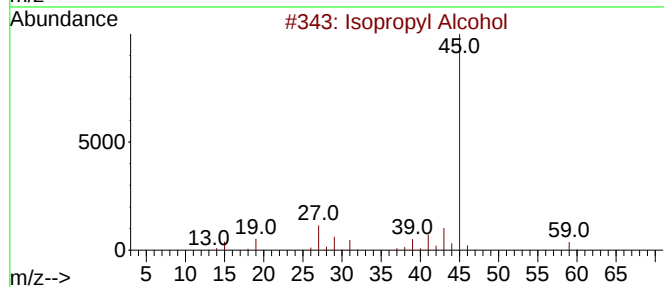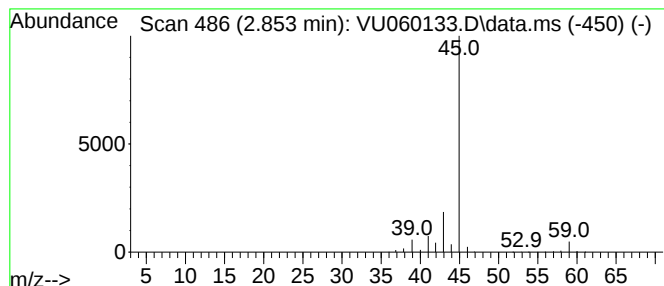

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060133.D
Acq On : 24 Jul 2024 00:03
Operator : MD/SY
Sample : P3300-25
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.447	11.6	ug/L	838215	1	6.242	360287	5.0
Isopropyl Alcohol	2.853	150.7	ug/L	10859600	1	6.242	360287	5.0