

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060135.D
 Acq On : 24 Jul 2024 00:50
 Operator : MD/SY
 Sample : P3300-23
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU060135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	347	360	382	rVB	672649	1089182	11.15%	7.367%
2	2.560	383	395	408	rBV	101673	163101	1.67%	1.103%
3	2.640	408	420	450	rBV	37753	118820	1.22%	0.804%
4	2.846	450	484	603	rBV2	1028152	9772320	100.00%	66.101%
5	4.631	1029	1039	1063	rBV	56816	170765	1.75%	1.155%
6	5.055	1156	1171	1191	rBV	88127	201345	2.06%	1.362%
7	5.718	1357	1377	1400	rBV2	180574	466088	4.77%	3.153%
8	6.242	1528	1540	1569	rBV	175541	342541	3.51%	2.317%
9	6.682	1665	1677	1698	rBV	109087	213454	2.18%	1.444%
10	7.894	2041	2054	2067	rBV	206278	366235	3.75%	2.477%
11	7.965	2067	2076	2103	rVB	55123	102004	1.04%	0.690%
12	8.631	2272	2283	2317	rBV	215379	435123	4.45%	2.943%
13	9.412	2513	2526	2549	rBV	268771	451261	4.62%	3.052%
14	10.749	2931	2942	2960	rBV2	93942	151415	1.55%	1.024%
15	11.807	3258	3271	3293	rBV	241368	402557	4.12%	2.723%
16	12.187	3375	3389	3404	rBV	201657	337814	3.46%	2.285%




Sum of corrected areas: 14784025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060135.D
Acq On : 24 Jul 2024 00:50
Operator : MD/SY
Sample : P3300-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

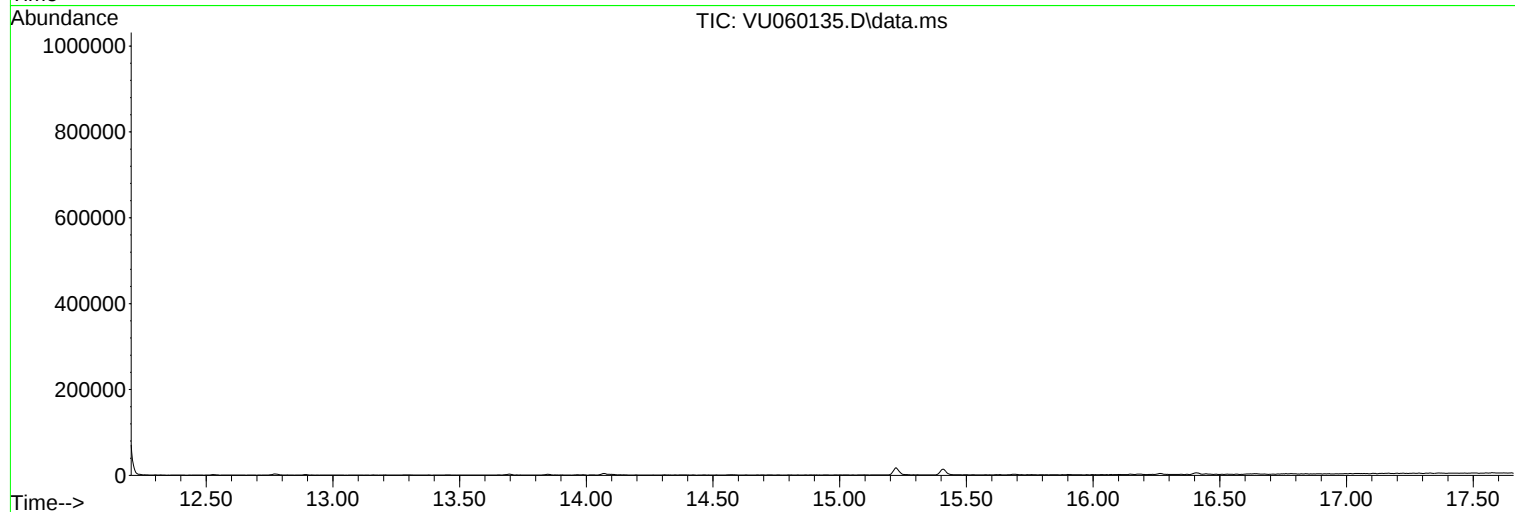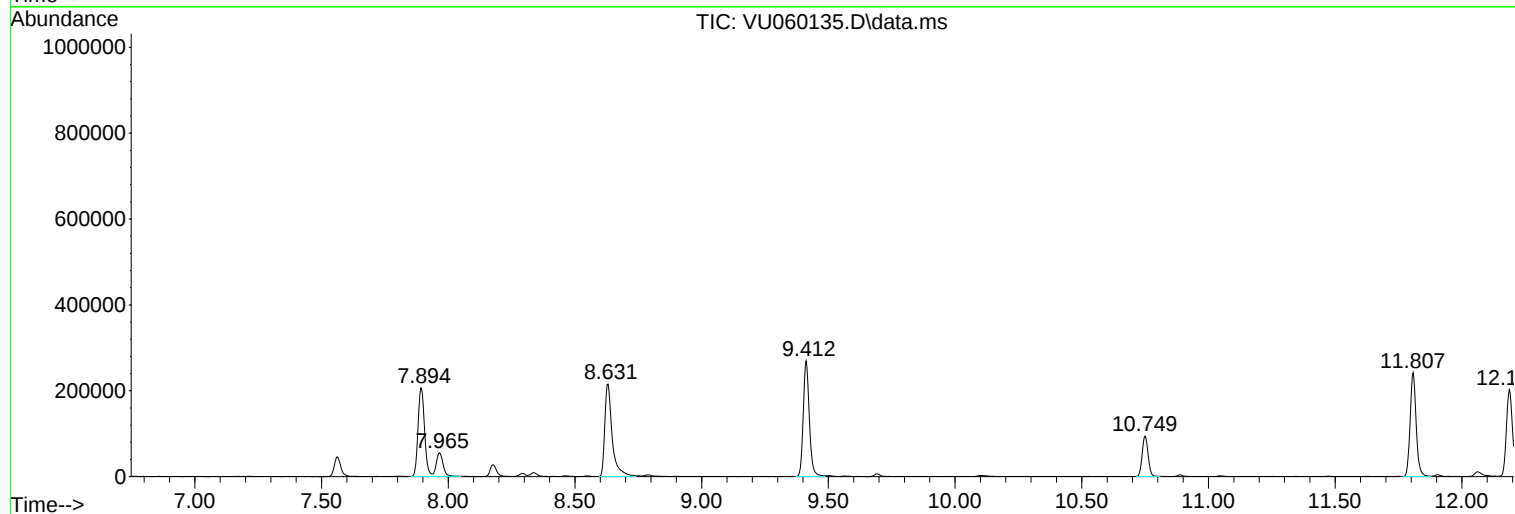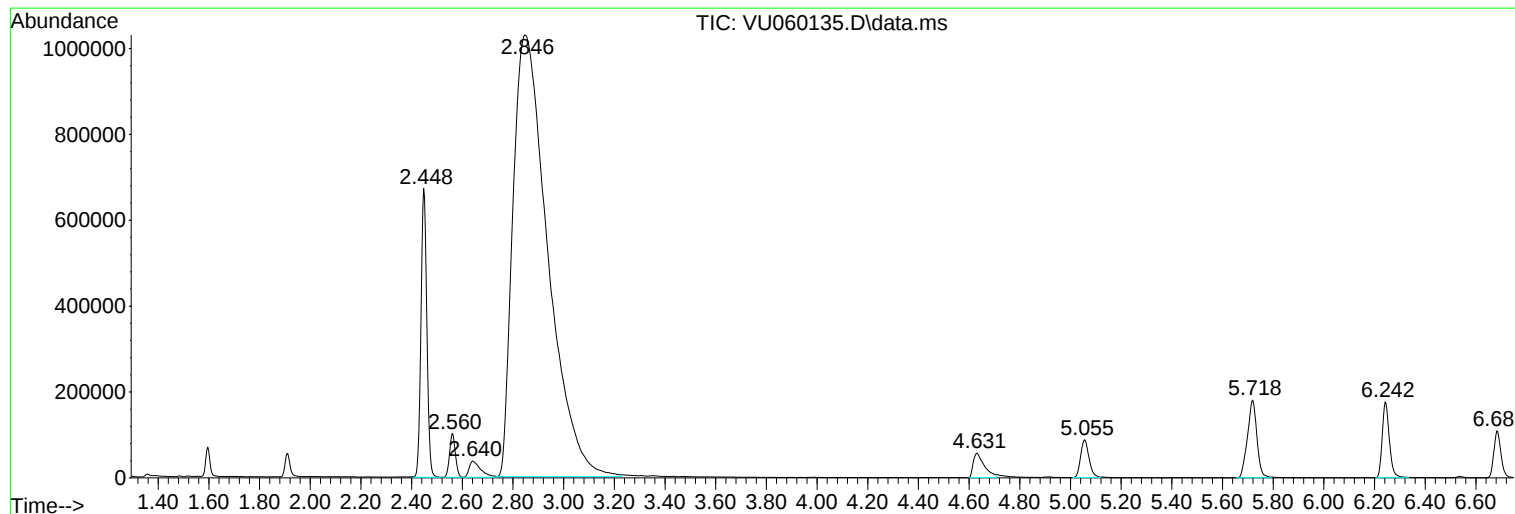

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060135.D
Acq On : 24 Jul 2024 00:50
Operator : MD/SY
Sample : P3300-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD2







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	15.90 ug/L	1089180	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	91
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	78
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	59
4			Acetyl chloride	78	C2H3ClO	000075-36-5	9
5			2-Chloroethanol	80	C2H5ClO	000107-07-3	4

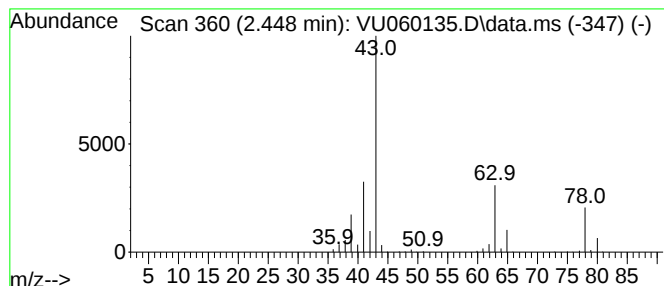

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060135.D
Acq On : 24 Jul 2024 00:50
Operator : MD/SY
Sample : P3300-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.846	142.65 ug/L	9772320	1,4-Difluorobenzene	6.242

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol		60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol		60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol		60	C3H8O	000067-63-0	56
4	Isopropyl Alcohol		60	C3H8O	000067-63-0	43
5	Isopropyl Alcohol		60	C3H8O	000067-63-0	9

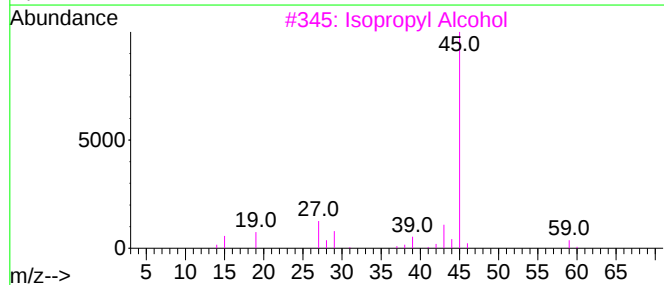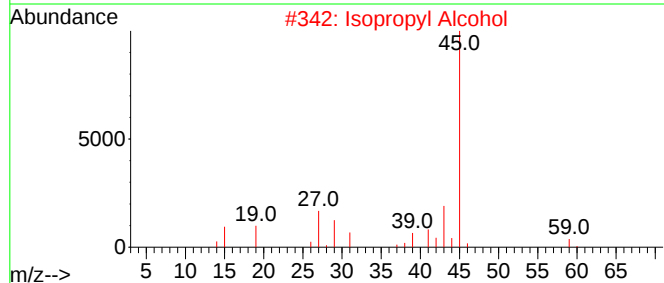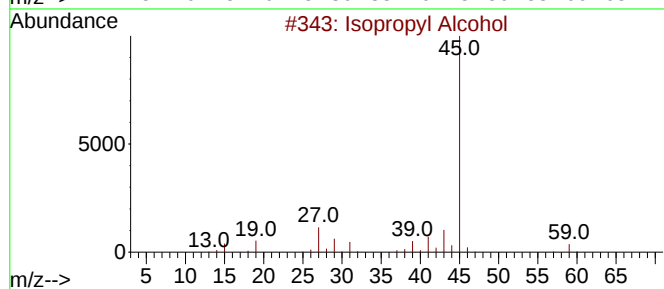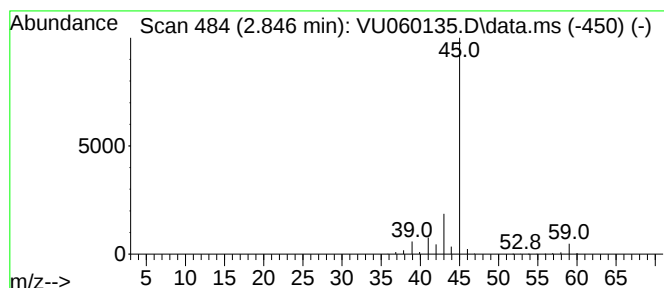

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060135.D
Acq On : 24 Jul 2024 00:50
Operator : MD/SY
Sample : P3300-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	15.9	ug/L	1089180	1	6.242	342541	5.0
Isopropyl Alcohol	2.846	142.7	ug/L	9772320	1	6.242	342541	5.0