

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060141.D
 Acq On : 24 Jul 2024 03:13
 Operator : MD/SY
 Sample : P3300-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G90

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU060141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	107	rBV3	87691	109411	1.01%	0.683%
2	2.448	347	360	381	rVB	563000	907451	8.41%	5.666%
3	2.560	381	395	412	rBV	99892	166966	1.55%	1.042%
4	2.846	449	484	595	rBV2	1116432	10793427	100.00%	67.387%
5	4.657	1028	1047	1079	rBV2	163931	505284	4.68%	3.155%
6	5.055	1155	1171	1195	rBV	91292	217215	2.01%	1.356%
7	5.718	1358	1377	1410	rBV2	182734	483311	4.48%	3.017%
8	6.242	1528	1540	1561	rBV	177521	343109	3.18%	2.142%
9	6.538	1621	1632	1650	rBV2	58293	108738	1.01%	0.679%
10	6.685	1664	1678	1699	rBV	109269	218143	2.02%	1.362%
11	7.891	2040	2053	2069	rBV	209773	369952	3.43%	2.310%
12	8.631	2272	2283	2323	rBV	224930	454946	4.22%	2.840%
13	9.412	2512	2526	2556	rBV	266870	450627	4.18%	2.813%
14	10.750	2928	2942	2961	rBV	96623	157625	1.46%	0.984%
15	11.807	3259	3271	3292	rBV	236912	391916	3.63%	2.447%
16	12.187	3377	3389	3408	rBV	203182	339004	3.14%	2.117%




Sum of corrected areas: 16017125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060141.D
Acq On : 24 Jul 2024 03:13
Operator : MD/SY
Sample : P3300-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

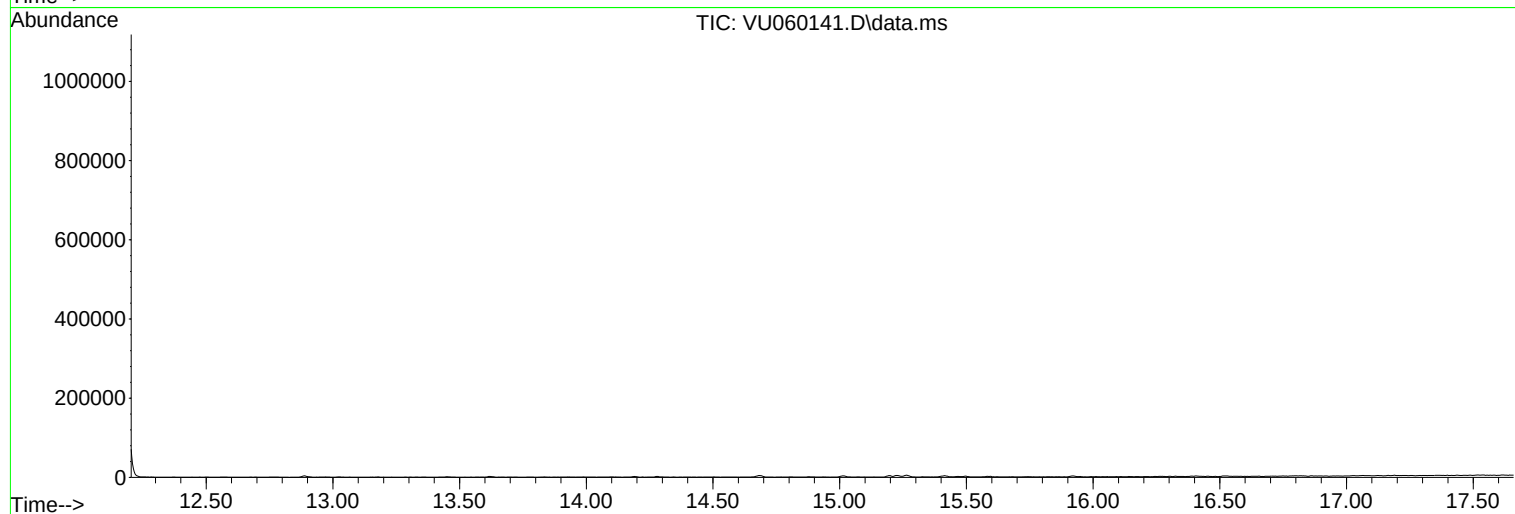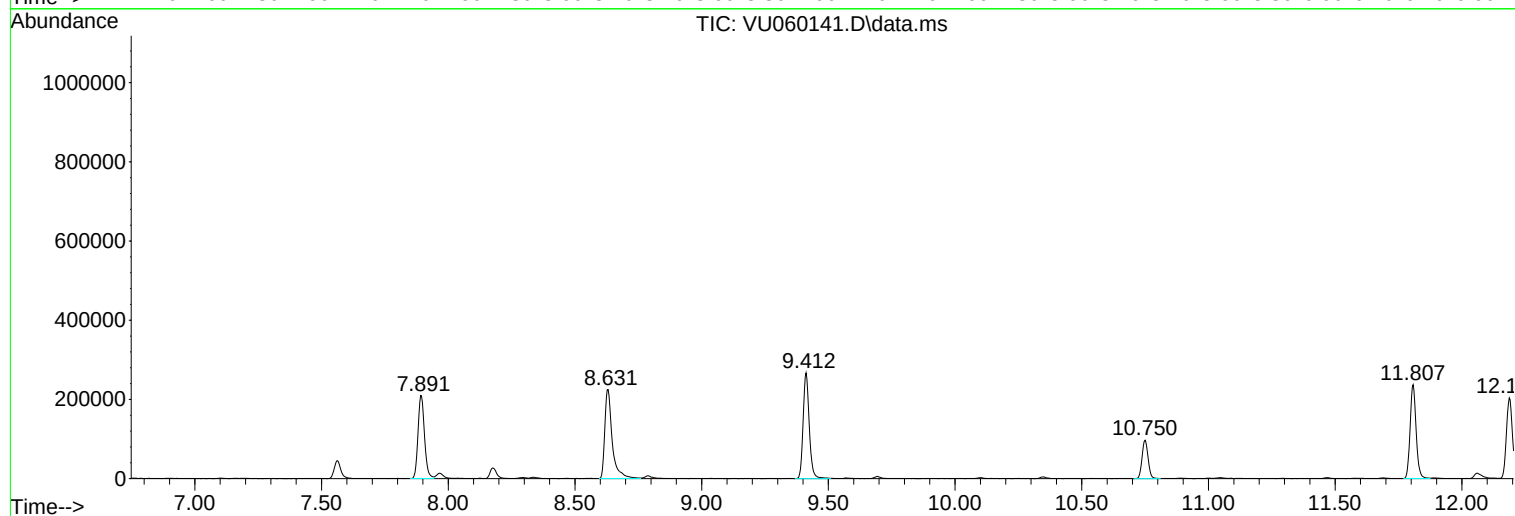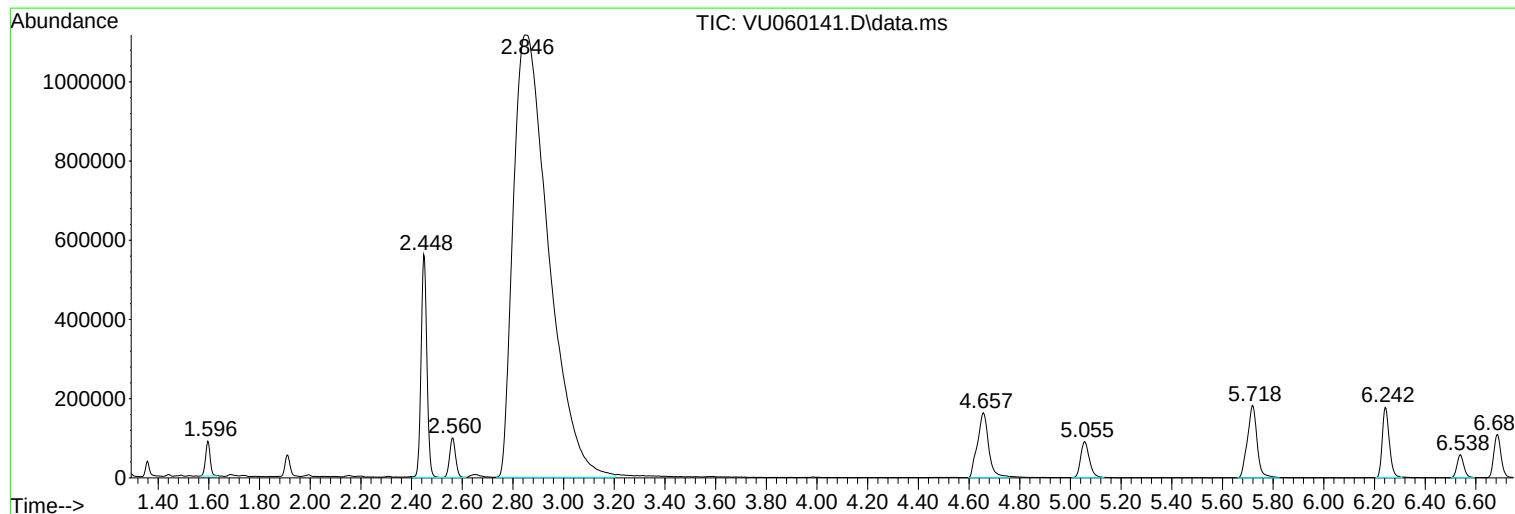

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060141.D
Acq On : 24 Jul 2024 03:13
Operator : MD/SY
Sample : P3300-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G90










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	13.22 ug/L	907451	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	91
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	50
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	42
4			Isopropylsulfonyl chloride	142	C3H7ClO2S	010147-37-2	9
5			Acetyl chloride	78	C2H3ClO	000075-36-5	9

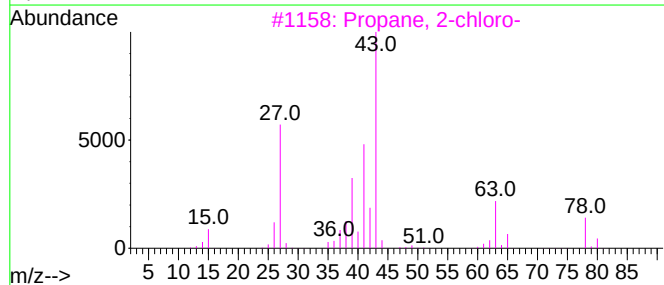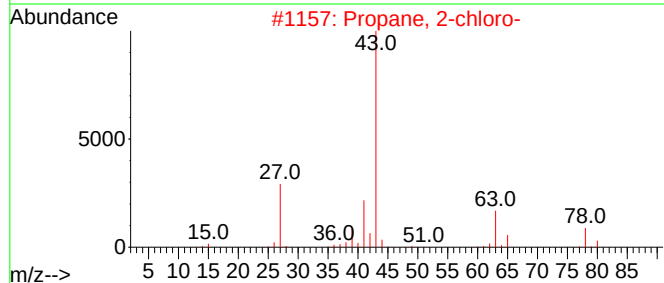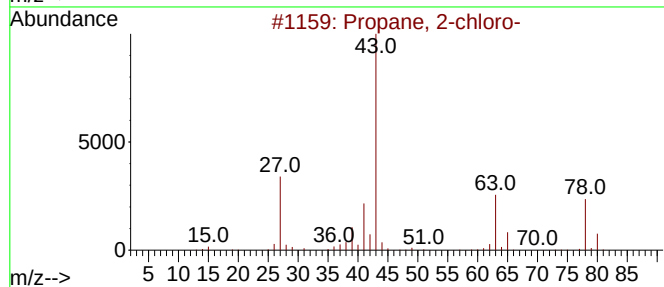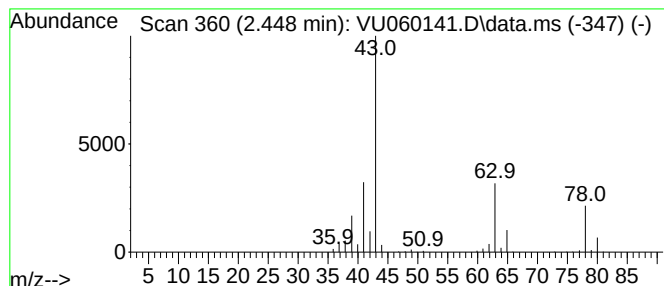

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060141.D
Acq On : 24 Jul 2024 03:13
Operator : MD/SY
Sample : P3300-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G90










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.846	157.29 ug/L	10793400	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

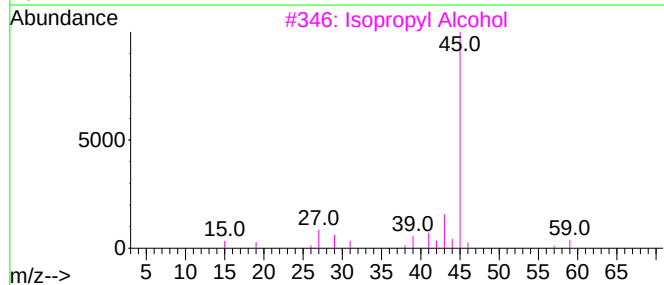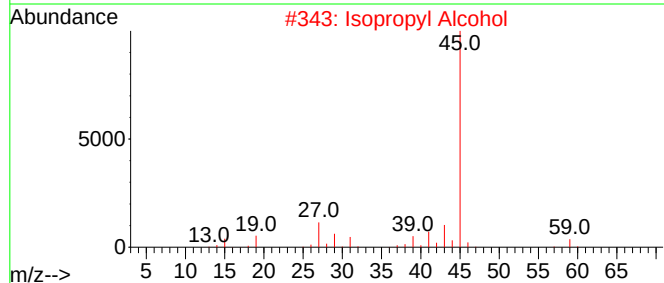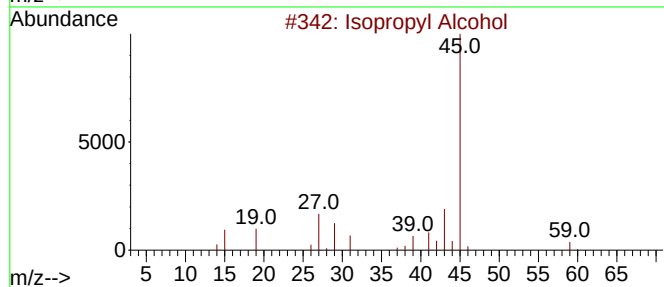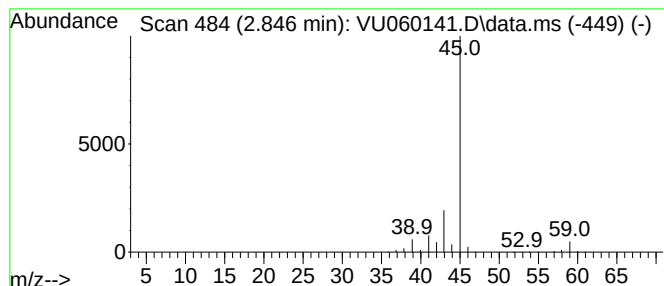

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060141.D
Acq On : 24 Jul 2024 03:13
Operator : MD/SY
Sample : P3300-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	13.2	ug/L	907451	1	6.242	343109	5.0
Isopropyl Alcohol	2.846	157.3	ug/L	10793400	1	6.242	343109	5.0