

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060142.D
 Acq On : 24 Jul 2024 03:37
 Operator : MD/SY
 Sample : P3300-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G65

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	347	360	381	rVB	353664	579558	5.50%	3.854%
2	2.560	381	395	410	rBV	105869	174656	1.66%	1.161%
3	2.849	448	485	597	rBV2	1092721	10539360	100.00%	70.082%
4	4.628	1028	1038	1074	rBV	60673	201249	1.91%	1.338%
5	5.055	1156	1171	1201	rBV2	98085	243333	2.31%	1.618%
6	5.718	1358	1377	1410	rBV2	189814	518863	4.92%	3.450%
7	6.242	1528	1540	1564	rBV	169292	327418	3.11%	2.177%
8	6.682	1665	1677	1697	rBV	116350	231887	2.20%	1.542%
9	7.891	2041	2053	2068	rBV	228204	394547	3.74%	2.624%
10	8.631	2271	2283	2317	rBV	241032	483938	4.59%	3.218%
11	9.412	2514	2526	2564	rBV	258585	429730	4.08%	2.858%
12	10.750	2926	2942	2957	rBV2	104681	165485	1.57%	1.100%
13	11.807	3257	3271	3292	rBV	231169	380947	3.61%	2.533%
14	12.187	3377	3389	3413	rVB	221809	367605	3.49%	2.444%




Sum of corrected areas: 15038576

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060142.D
Acq On : 24 Jul 2024 03:37
Operator : MD/SY
Sample : P3300-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

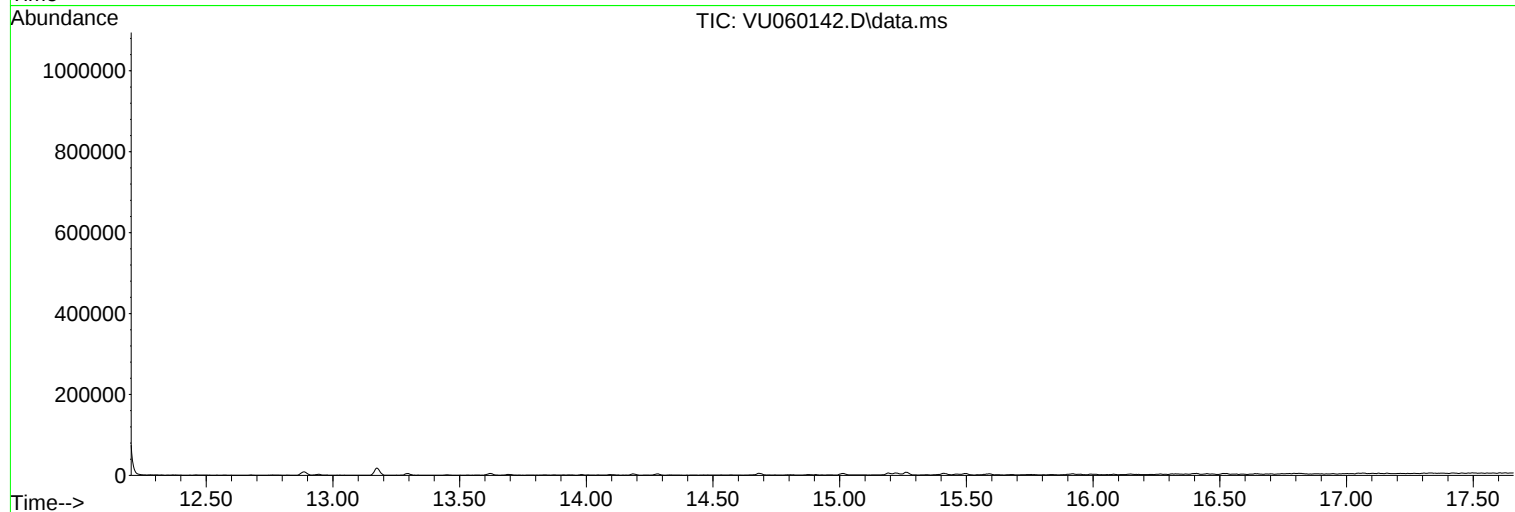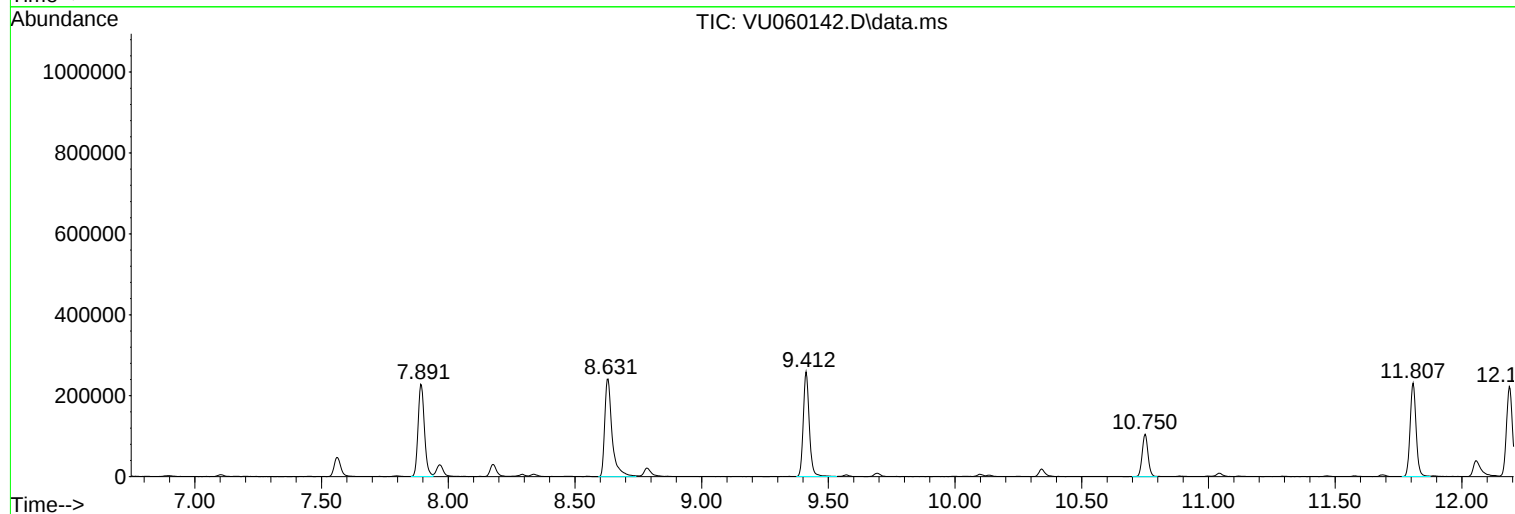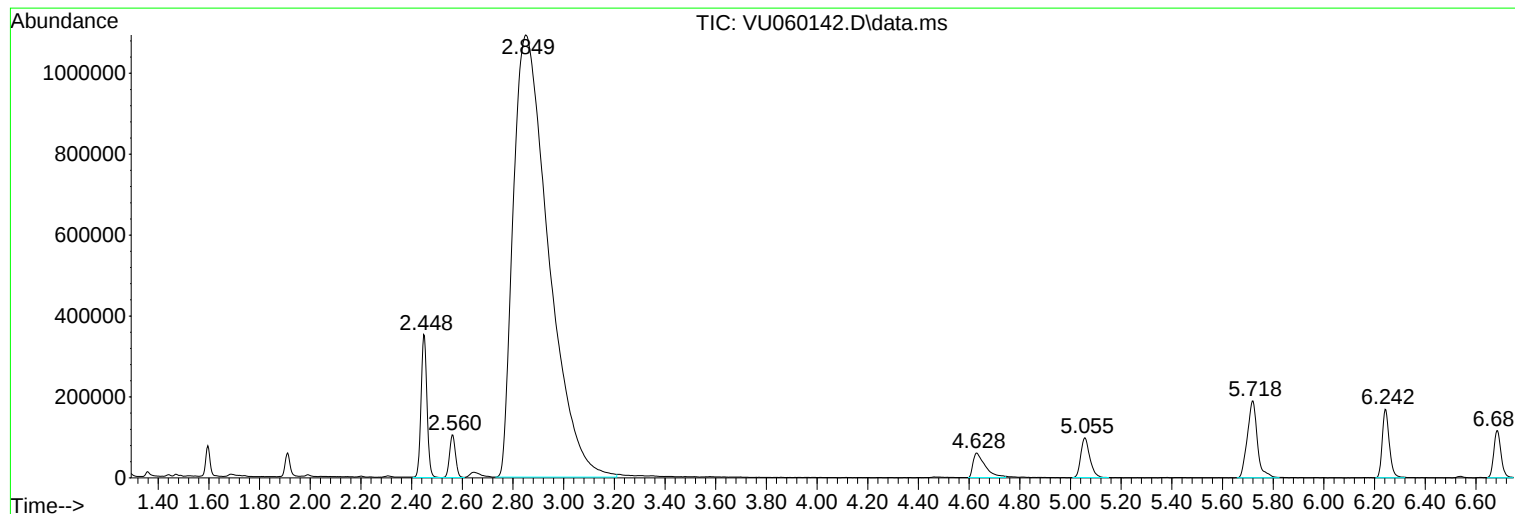

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060142.D
Acq On : 24 Jul 2024 03:37
Operator : MD/SY
Sample : P3300-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G65







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	8.85 ug/L	579558	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	50
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	42
4	Acetyl chloride			78	C2H3ClO	000075-36-5	9
5	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9

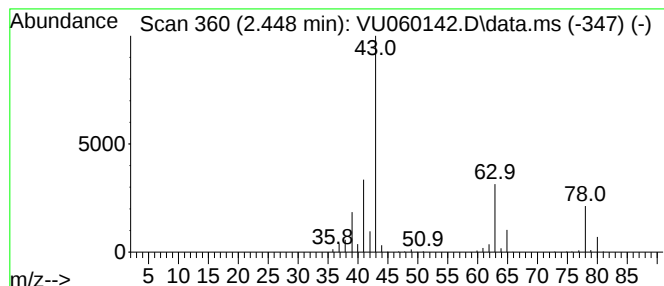

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060142.D
Acq On : 24 Jul 2024 03:37
Operator : MD/SY
Sample : P3300-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G65










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.849	160.95 ug/L	10539400	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	43
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

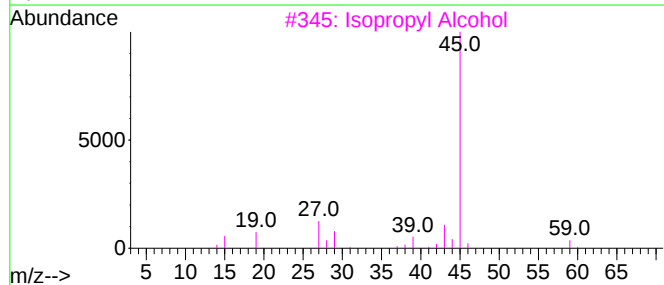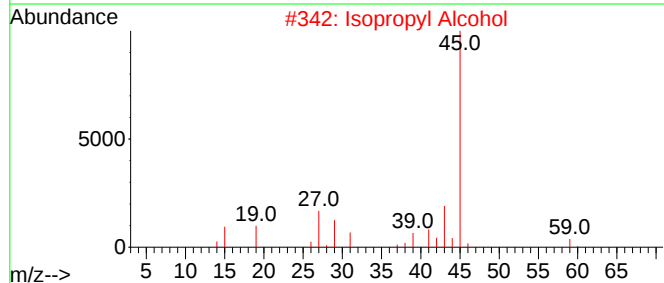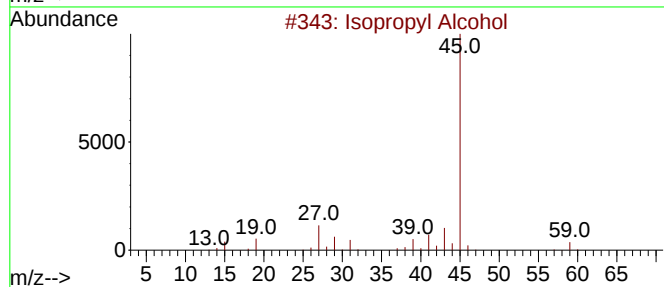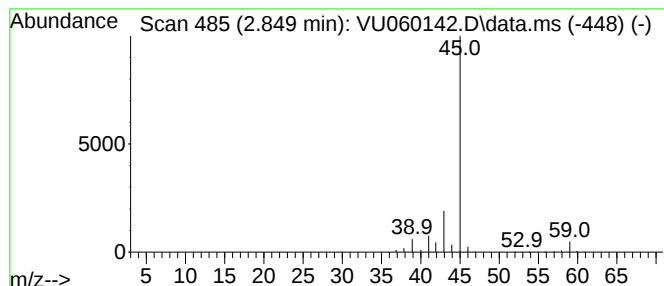

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060142.D
Acq On : 24 Jul 2024 03:37
Operator : MD/SY
Sample : P3300-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	8.8	ug/L	579558	1	6.242	327418	5.0
Isopropyl Alcohol	2.849	160.9	ug/L	10539400	1	6.242	327418	5.0