

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
 Data File : VU060143.D
 Acq On : 24 Jul 2024 04:01
 Operator : MD/SY
 Sample : P3300-26
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GE9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.447	347	360	380	rVB	596228	974085	9.67%	6.530%
2	2.560	384	395	408	rBV	100791	163123	1.62%	1.094%
3	2.644	408	421	449	rBV2	56612	175244	1.74%	1.175%
4	2.846	450	484	597	rVV2	1060648	10068386	100.00%	67.494%
5	4.627	1028	1038	1073	rBV	53565	175564	1.74%	1.177%
6	5.055	1157	1171	1192	rBV	90668	209011	2.08%	1.401%
7	5.717	1358	1377	1405	rBV2	183090	474471	4.71%	3.181%
8	6.242	1528	1540	1566	rBV	169747	331131	3.29%	2.220%
9	6.682	1664	1677	1707	rBV	107775	214793	2.13%	1.440%
10	7.894	2040	2054	2067	rBV	215062	375817	3.73%	2.519%
11	8.630	2271	2283	2320	rBV2	211170	435391	4.32%	2.919%
12	9.412	2514	2526	2551	rBV	261694	440632	4.38%	2.954%
13	10.749	2930	2942	2957	rBV	93788	150806	1.50%	1.011%
14	11.807	3258	3271	3293	rBV	236679	387717	3.85%	2.599%
15	12.187	3377	3389	3412	rBV	204225	341226	3.39%	2.287%




Sum of corrected areas: 14917397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060143.D
Acq On : 24 Jul 2024 04:01
Operator : MD/SY
Sample : P3300-26
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

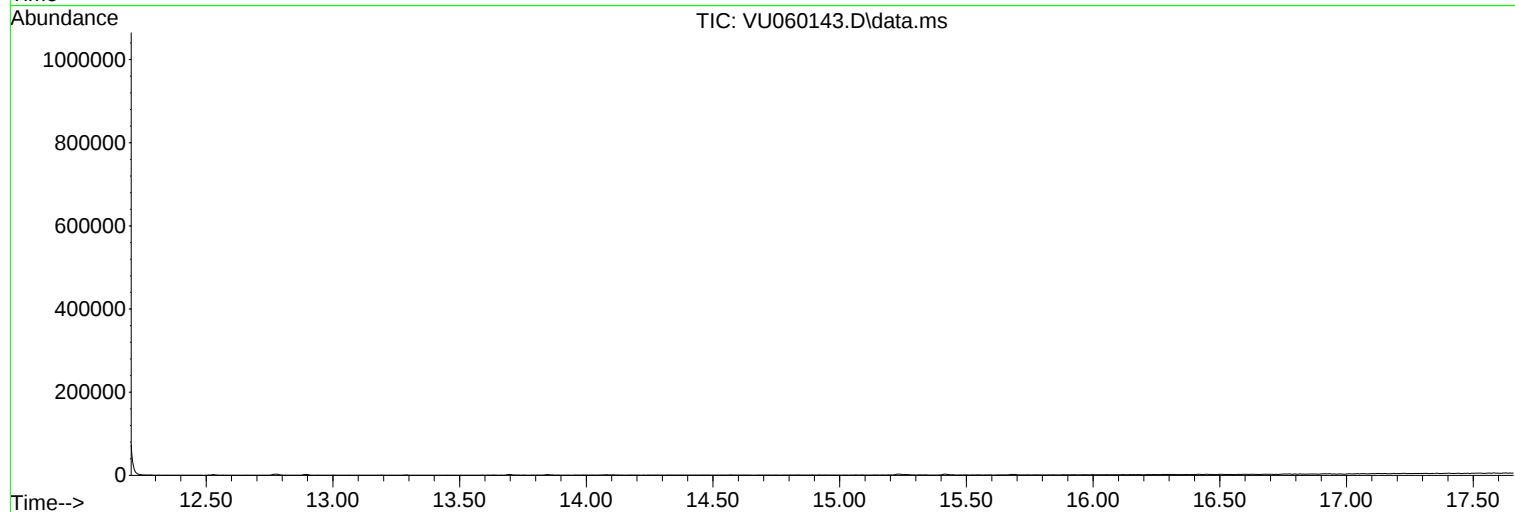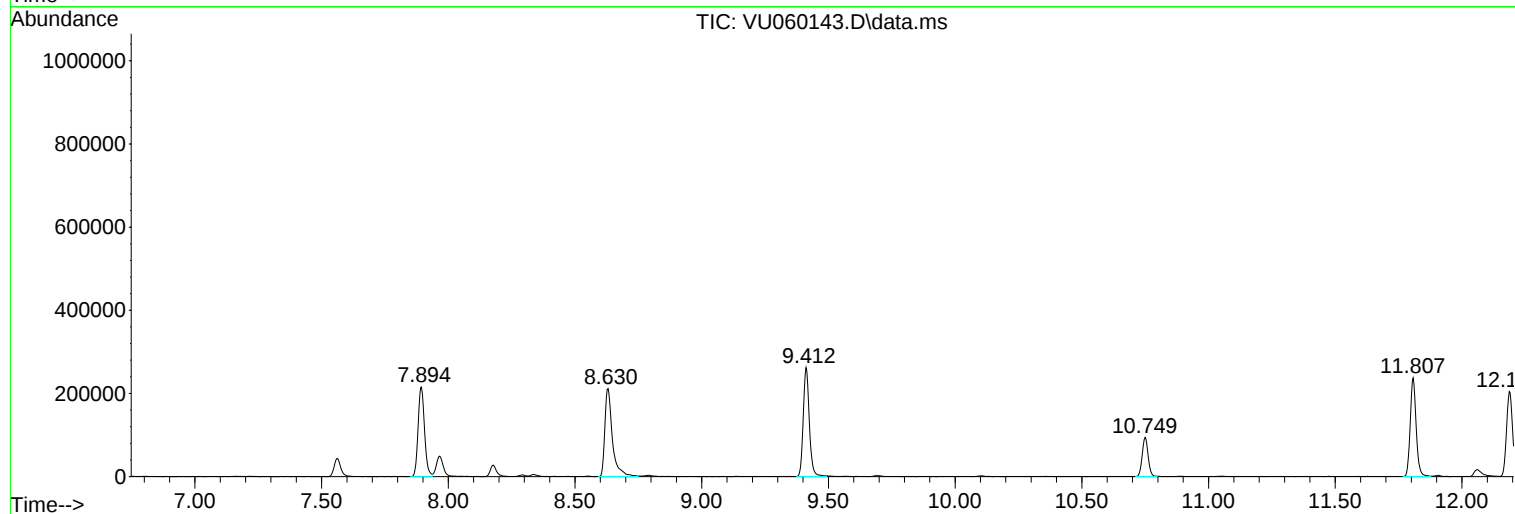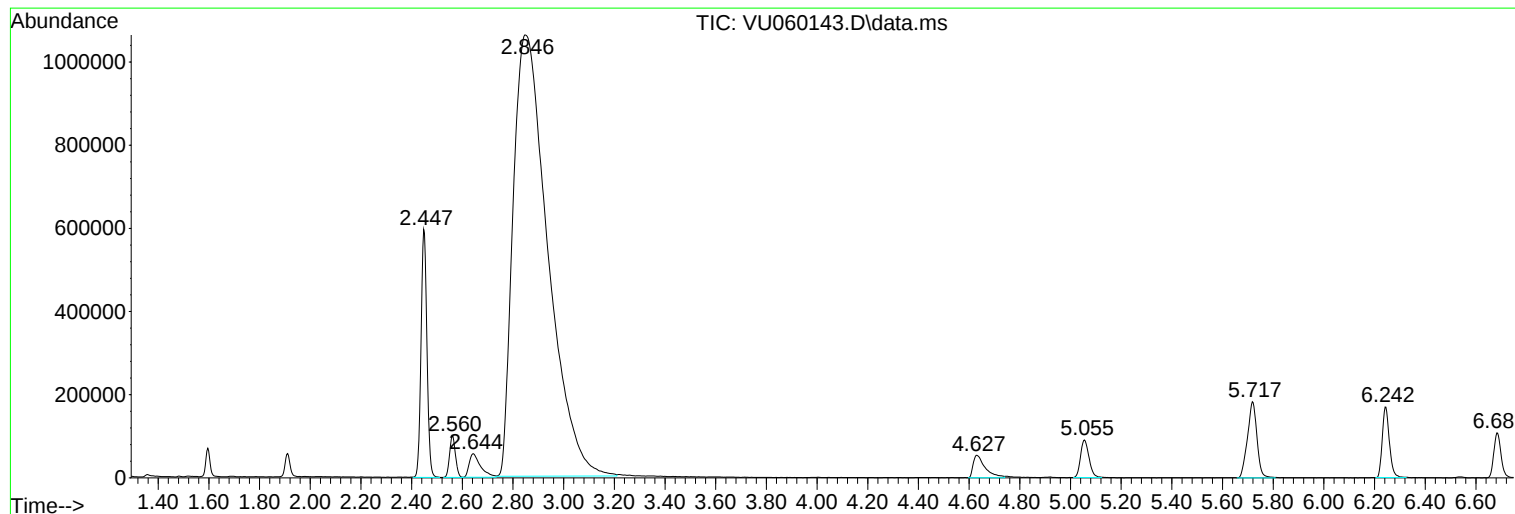

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060143.D
Acq On : 24 Jul 2024 04:01
Operator : MD/SY
Sample : P3300-26
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE9









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.447	14.71 ug/L	974085	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	50
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	50
4	Acetyl chloride			78	C2H3ClO	000075-36-5	9
5	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9

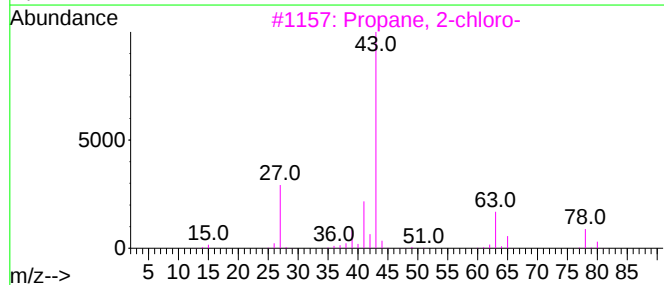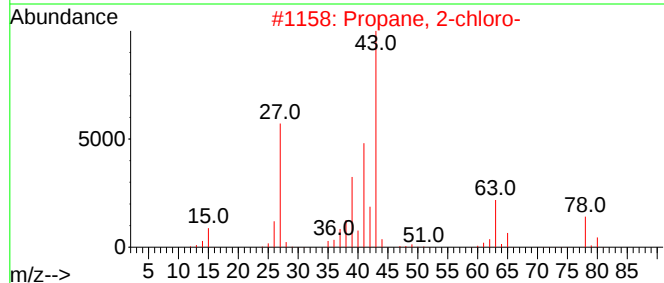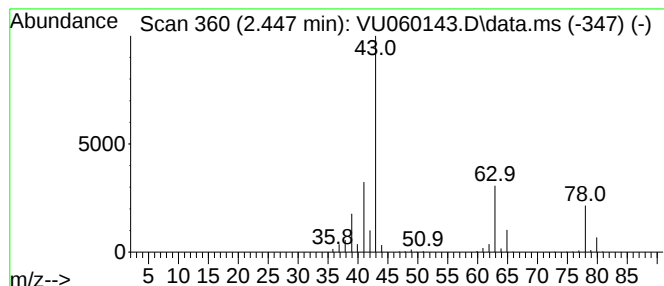

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060143.D
Acq On : 24 Jul 2024 04:01
Operator : MD/SY
Sample : P3300-26
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.846	152.03 ug/L	10068400	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	43
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

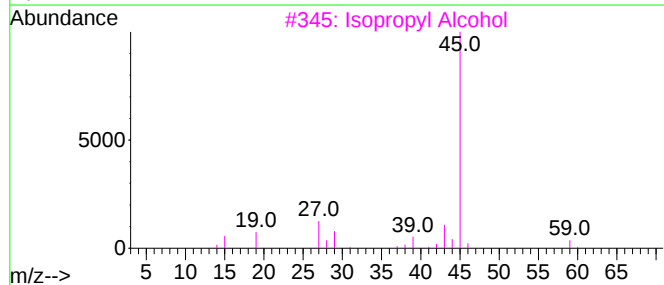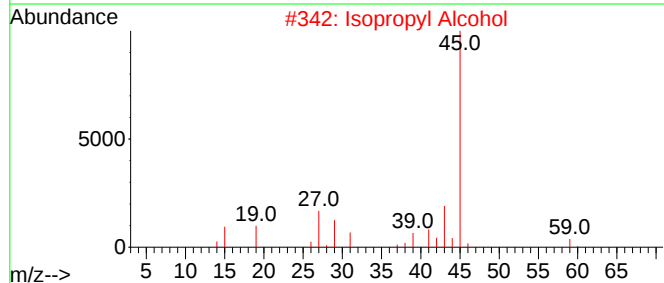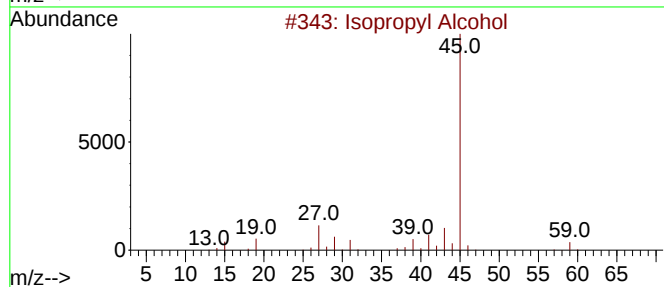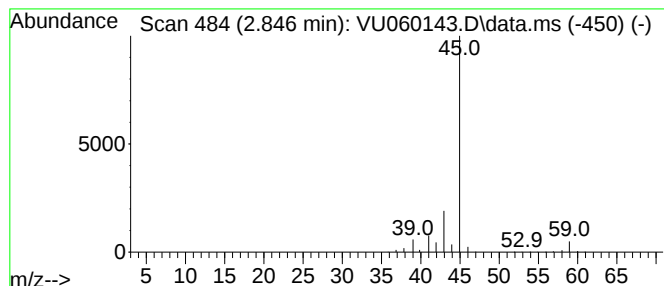

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060143.D
Acq On : 24 Jul 2024 04:01
Operator : MD/SY
Sample : P3300-26
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.447	14.7	ug/L	974085	1	6.242	331131	5.0
Isopropyl Alcohol	2.846	152.0	ug/L	10068400	1	6.242	331131	5.0