
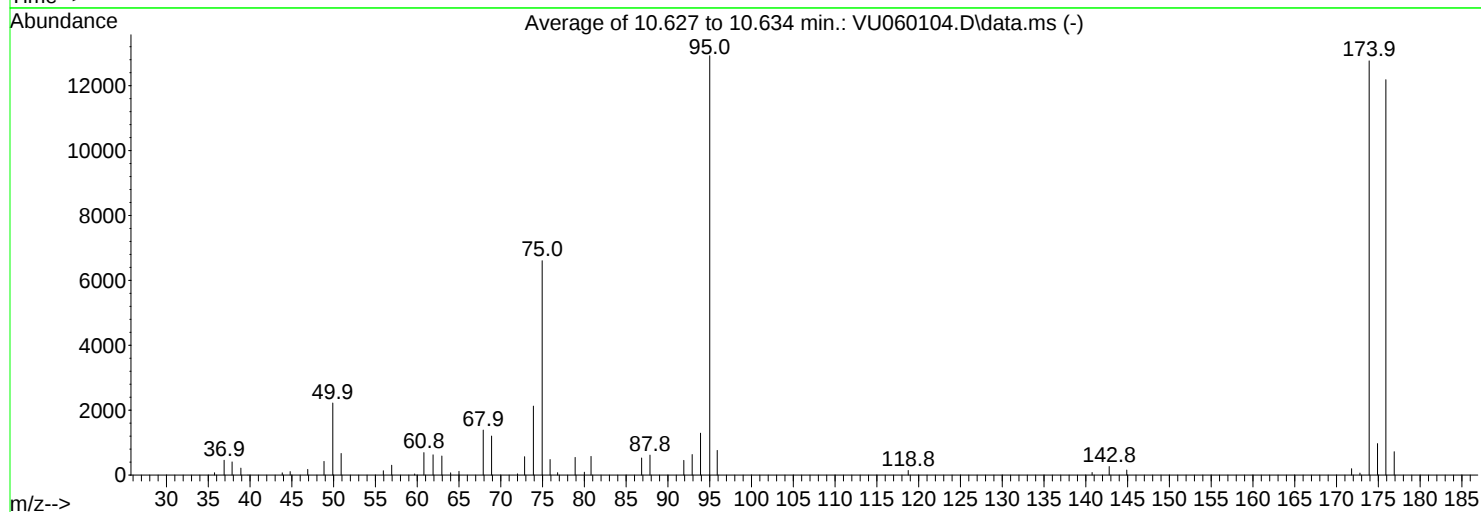


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072324\
Data File : VU060104.D
Acq On : 23 Jul 2024 09:47
Operator : MD/SY
Sample : BFB177
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB177

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jul 26 23:14:26 2024

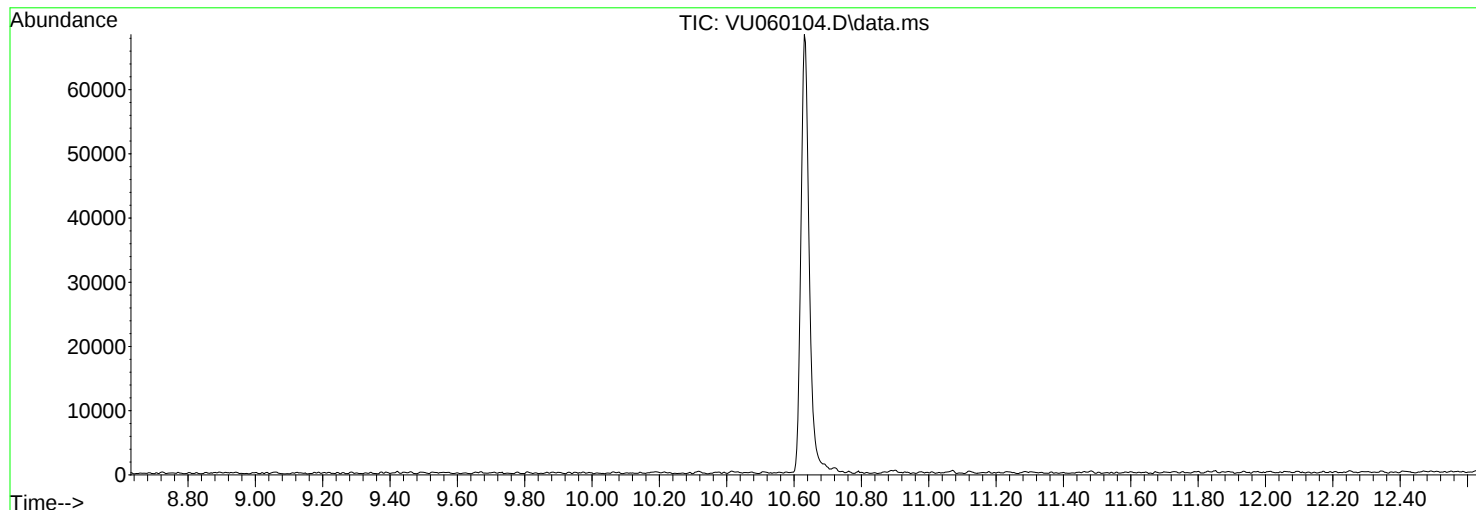

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	2220	PASS
75	95	30	80	51.1	6606	PASS
95	95	100	100	100.0	12923	PASS
96	95	5	9	5.9	760	PASS
173	174	0.00	2	0.5	62	PASS
174	95	50	120	98.8	12765	PASS
175	174	5	9	7.6	970	PASS
176	174	95	101	95.4	12184	PASS
177	176	5	9	5.9	720	PASS

Scan 2893 (10.592 min): VU060104.D\data.ms
BFB177

m/z	Abundance
39.80	155.0
43.80	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
35.80	111.0
36.90	441.0
37.80	445.0
38.90	206.0
39.80	116.0
43.90	314.0
44.80	176.0
46.90	187.0
48.90	402.0
49.90	2077.0
50.90	670.0
56.00	134.0
57.00	233.0
60.80	660.0
61.90	561.0
62.90	559.0
64.00	104.0
65.10	116.0
67.90	1367.0
68.90	1162.0
72.90	516.0
73.90	1967.0
74.90	6166.0
75.90	457.0
76.80	104.0
78.90	503.0
80.80	497.0
86.90	556.0
87.80	618.0
91.90	459.0
92.90	587.0
93.90	1188.0
95.00	12294.0
95.90	793.0
118.80	127.0
142.80	239.0
144.90	168.0
171.80	196.0
172.80	187.0
173.90	12301.0
174.90	853.0
175.90	11223.0
176.90	676.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
35.70	108.0
36.90	480.0
37.90	410.0
38.90	208.0
39.80	159.0
43.90	305.0
44.80	147.0
46.90	171.0
48.80	443.0
49.90	2312.0
50.90	693.0
55.90	133.0
57.00	323.0
60.80	749.0
61.90	645.0
63.00	603.0
64.00	103.0
65.00	103.0
67.90	1435.0
68.90	1250.0
72.90	585.0
73.90	2183.0
74.90	6827.0
75.90	493.0
76.80	118.0
78.90	576.0
80.00	118.0
80.80	592.0
86.80	535.0
87.80	635.0
91.90	471.0
92.90	648.0
93.90	1314.0
95.00	13362.0
95.90	783.0
118.70	144.0
140.70	115.0
142.80	288.0
144.90	169.0
171.80	209.0
173.90	13284.0
174.90	996.0
175.90	12602.0
176.90	726.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
36.90	449.0
37.90	362.0
38.90	227.0
39.70	192.0
43.90	336.0
46.90	163.0
48.80	418.0
49.90	2272.0
50.90	633.0
55.90	133.0
56.90	355.0
59.70	102.0
60.80	669.0
61.90	668.0
63.00	602.0
64.90	129.0
67.90	1360.0
68.90	1196.0
72.00	115.0
72.80	599.0
73.90	2227.0
75.00	6824.0
75.90	491.0
78.90	556.0
80.00	148.0
80.80	637.0
86.80	488.0
87.90	595.0
91.90	430.0
92.90	663.0
93.90	1372.0
95.00	13113.0
95.90	703.0
118.70	154.0
140.80	126.0
142.80	263.0
144.90	127.0
171.80	185.0
173.90	12711.0
174.90	1061.0
175.90	12726.0
176.90	758.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177