

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072418\
 Data File : VU025620.D
 Acq On : 24 Jul 2018 11:08
 Operator : MD/SY
 Sample : VU0724WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 25 02:26:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 25 02:26:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	290051	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	271410	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	140781	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	96238	58.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	116.24%
7) Chloroethane-d5	1.68	69	80030	58.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	117.18%
11) 1,1-Dichloroethene-d2	2.27	63	144681	41.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.94%
21) 2-Butanone-d5	4.18	46	154768	121.07	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	121.07%
24) Chloroform-d	4.65	84	204003	55.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.62%
26) 1,2-Dichloroethane-d4	5.31	65	141092	57.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.68%
32) Benzene-d6	5.35	84	403741	58.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	116.00%
36) 1,2-Dichloropropane-d6	6.33	67	126897	56.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	113.16%
41) Toluene-d8	7.57	98	383086	57.39	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	114.78%
43) trans-1,3-Dichloropropene-	7.85	79	65956	57.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	115.14%
47) 2-Hexanone-d5	8.31	63	109059	116.13	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.13%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	173149	55.20	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	110.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	162318	56.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.78%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	11.49	75	15340	6.128 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072418\
Data File : VU025620.D
Acq On : 24 Jul 2018 11:08
Operator : MD/SY
Sample : VU0724WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jul 25 02:26:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 25 02:26:32 2018
Response via : Initial Calibration

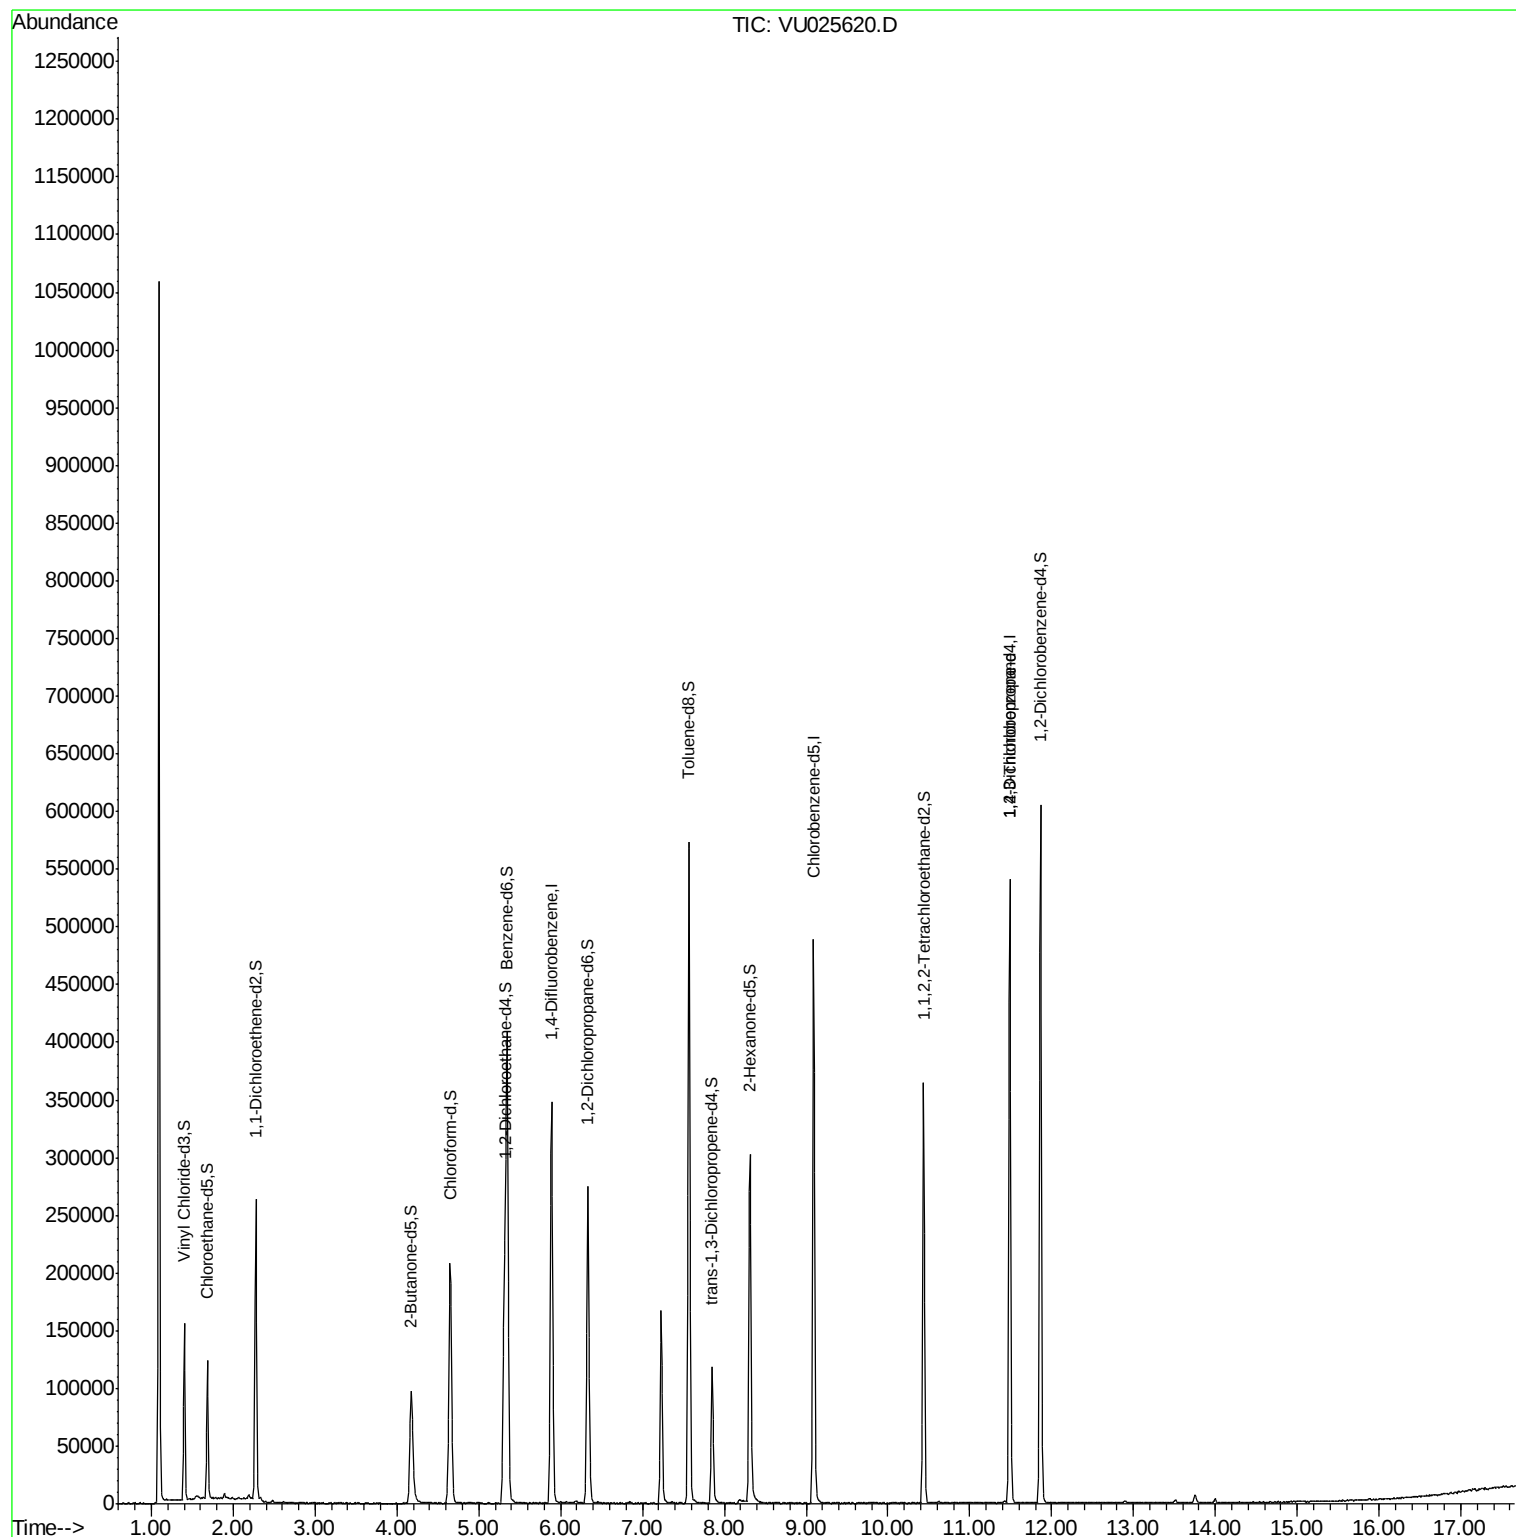

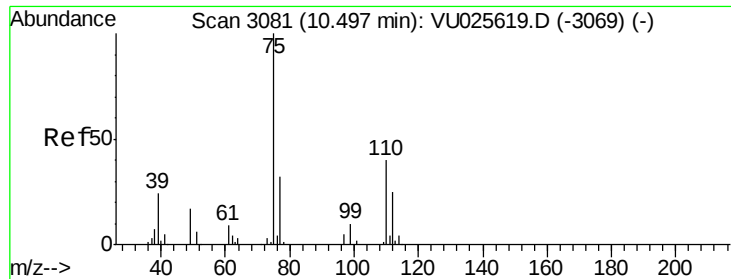

#59

1,2,3-Trichloropropane

Concen: 6.128 ug/L

RT: 11.49 min Scan# 3389

Delta R.T. 0.99 min

Lab File: VU025620.D

Acq: 24 Jul 2018 11:08

Instrument :

MSVOA_U


ClientSampleId :

Tot Ion: 75 Resp: 15340

Ion Ratio Lower Upper

75 100

77 38.6 25.8 38.8

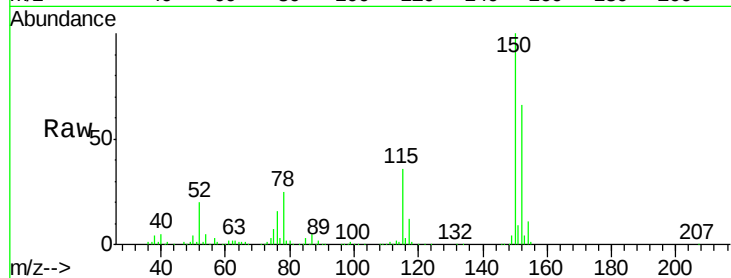

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 77.00 (76.70 to 77.70): VU0

