


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072418\
 Data File : VU025618.D
 Acq On : 24 Jul 2018 09:34
 Operator : MD/SY
 Sample : BFB49
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 04 04:39:04 2018

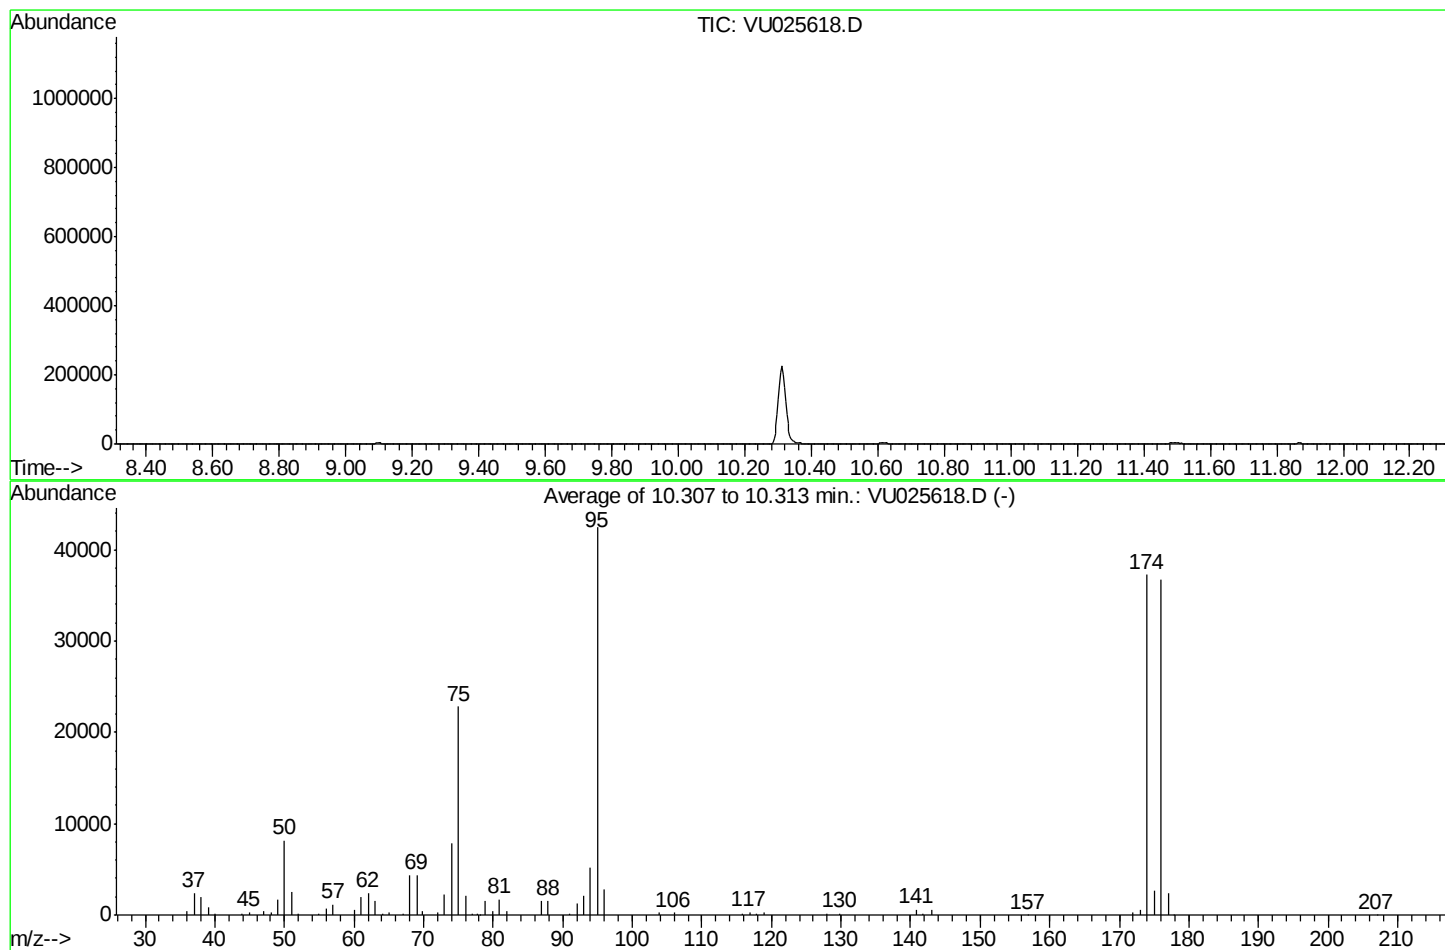

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	8185	PASS
75	95	30	80	53.7	22778	PASS
95	95	100	100	100.0	42442	PASS
96	95	5	9	6.6	2810	PASS
173	174	0.00	2	1.5	559	PASS
174	95	50	120	87.8	37272	PASS
175	174	5	9	7.1	2634	PASS
176	174	95	101	98.7	36789	PASS
177	176	5	9	6.5	2379	PASS

m/z	Abundance
43.90	528.0
207.00	230.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
35.90	465.0
37.00	2299.0
38.00	1696.0
39.00	723.0
39.90	147.0
43.90	745.0
44.90	259.0
47.00	488.0
48.10	330.0
49.00	1547.0
50.00	7965.0
51.00	2417.0
52.00	144.0
54.80	124.0
56.10	633.0
57.00	1044.0
60.00	571.0
61.00	2078.0
62.00	2290.0
63.00	1474.0
64.10	184.0
65.00	312.0
67.10	166.0
68.00	4145.0
69.00	4137.0
69.90	356.0
71.90	260.0
73.00	2122.0
74.00	7536.0
75.00	21760.0
76.00	1986.0
77.00	215.0
77.80	175.0
78.90	1396.0
79.90	442.0
80.90	1663.0
81.90	334.0
86.90	1596.0
87.90	1555.0
91.00	162.0
92.00	1101.0
93.00	1912.0
94.00	4963.0
95.00	40272.0
96.00	2765.0
103.80	220.0
106.00	242.0
115.90	156.0
116.90	296.0
117.80	116.0
118.90	353.0
128.00	192.0
129.90	220.0
140.90	600.0
141.80	123.0
143.00	469.0
172.00	351.0
173.10	509.0
174.00	34696.0
175.00	2656.0
176.00	33944.0
177.00	2372.0
207.00	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
35.90	496.0
37.00	2474.0
38.10	1944.0
39.00	816.0
39.90	151.0
43.90	796.0
44.90	331.0
46.90	446.0
48.10	349.0
49.00	1631.0
50.00	8436.0
51.10	2640.0
52.00	166.0
54.80	137.0
56.10	632.0
57.00	1156.0
60.00	596.0
61.00	2092.0
62.00	2455.0
63.00	1542.0
64.10	153.0
65.00	315.0
67.00	209.0
68.00	4506.0
69.00	4507.0
69.90	362.0
72.00	209.0
73.00	2279.0
74.00	8215.0
75.00	23528.0
76.00	2148.0
77.00	186.0
77.60	192.0
78.90	1526.0
79.90	496.0
80.90	1759.0
81.90	396.0
86.90	1660.0
87.90	1682.0
90.90	164.0
92.00	1261.0
93.00	2178.0
94.00	5395.0
95.00	43768.0
96.00	2924.0
103.80	268.0
106.00	281.0
115.80	184.0
116.90	369.0
117.70	154.0
118.90	351.0
128.00	188.0
129.80	200.0
140.90	652.0
141.80	121.0
143.00	564.0
171.90	335.0
173.10	592.0
174.00	38576.0
175.00	2731.0
176.00	38176.0
177.00	2434.0
207.00	282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
35.90	428.0
37.00	2404.0
38.10	2072.0
39.00	867.0
40.00	146.0
43.90	665.0
44.90	351.0
46.90	373.0
48.10	317.0
49.00	1673.0
50.00	8156.0
51.10	2697.0
52.00	162.0
54.90	113.0
56.00	741.0
56.90	1216.0
60.00	472.0
61.00	1912.0
62.00	2465.0
63.00	1542.0
64.00	130.0
65.00	279.0
66.90	228.0
68.00	4529.0
69.00	4563.0
69.90	379.0
72.10	194.0
73.00	2181.0
74.00	7843.0
75.00	23048.0
76.00	2108.0
77.10	148.0
77.60	197.0
78.10	103.0
78.90	1542.0
79.90	478.0
80.90	1664.0
81.90	407.0
86.90	1490.0
87.90	1560.0
90.90	169.0
92.00	1266.0
93.00	2129.0
94.00	5114.0
95.00	43288.0
96.00	2743.0
103.80	303.0
106.00	294.0
115.70	183.0
116.90	380.0
117.80	197.0
118.80	341.0
128.00	142.0
129.80	195.0
140.90	597.0
143.00	655.0
156.90	124.0
171.90	350.0
173.10	578.0
174.00	38544.0
175.00	2517.0
176.00	38248.0
177.00	2332.0
177.80	104.0
207.00	272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49