

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072419\
 Data File : VU033387.D
 Acq On : 24 Jul 2019 11:42
 Operator : JC/SP
 Sample : VU0724WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0724WBL01

Quant Time: Jul 25 07:58:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U072219DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Jul 24 03:53:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.72	96	25256	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.30	95	7915	0.80	ug/l	0.00
Spiked Amount 1.000			Recovery	=	80.00%	
68) 1,2-Dichlorobenzene-d4	11.85	152	8358	0.82	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072419\
Data File : VU033387.D
Acq On : 24 Jul 2019 11:42
Operator : JC/SP
Sample : VU0724WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0724WBL01

Quant Time: Jul 25 07:58:54 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U072219DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Jul 24 03:53:19 2019
Response via : Initial Calibration

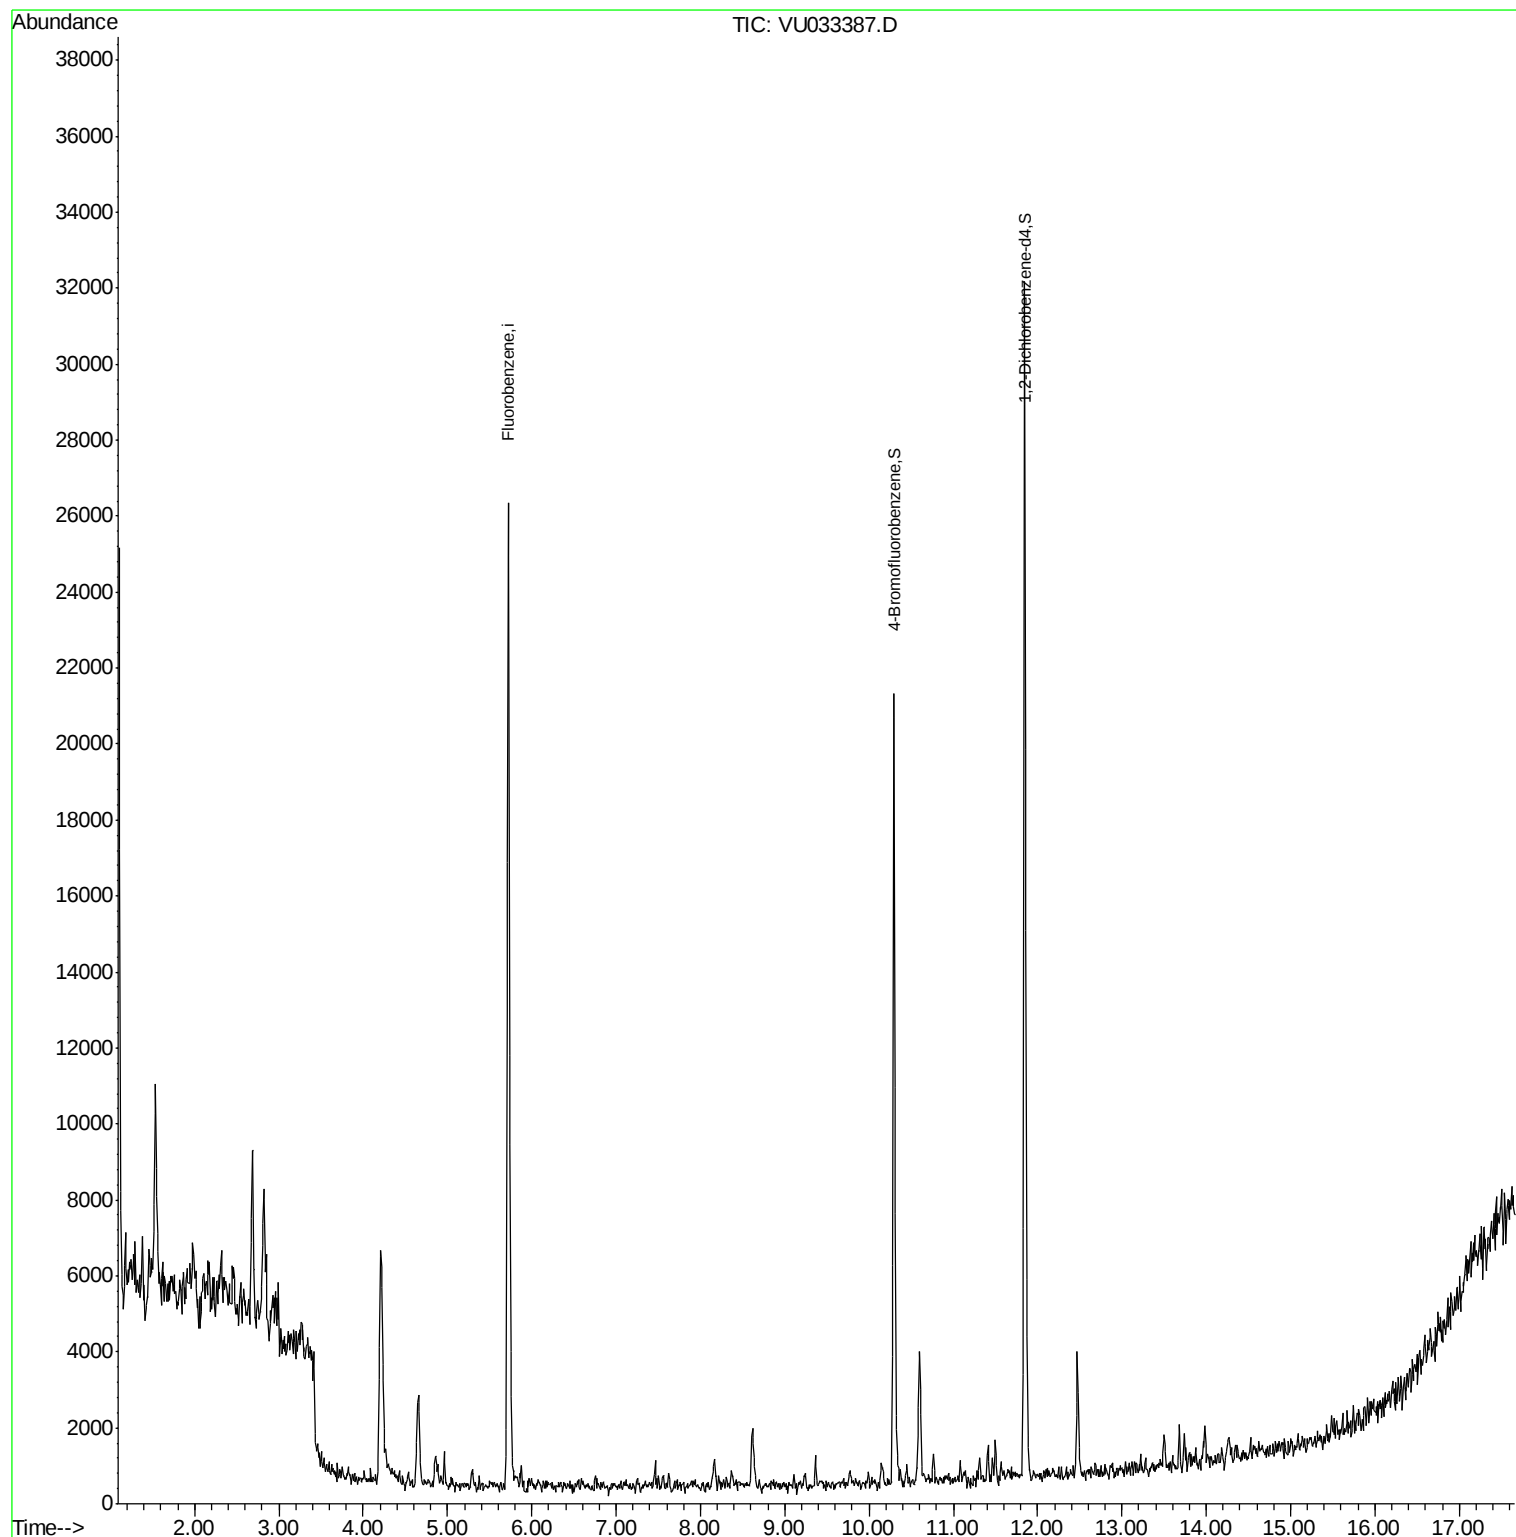

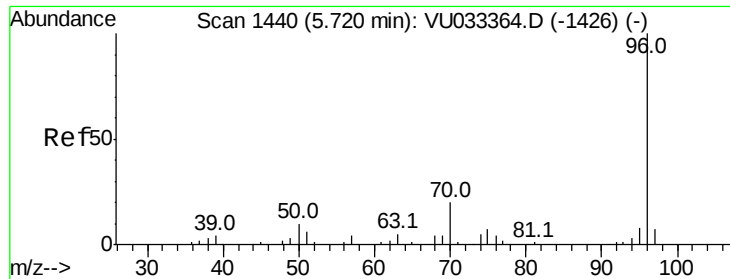

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.72 min Scan# 1440

Delta R.T. -0.00 min

Lab File: VU033387.D

Acq: 24 Jul 2019 11:42

Instrument :

MSVOA_U

ClientSampleId :

VU0724WBL01

Tot Ion: 96 Resp: 25256


Ion Ratio Lower Upper

96 100

70 19.4 16.4 24.6

95 9.5 6.7 10.1

97 6.0 0.0 0.0#



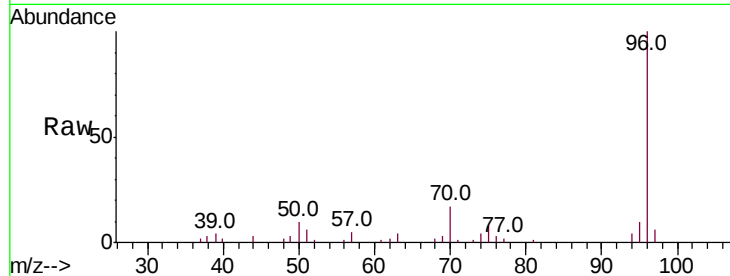


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

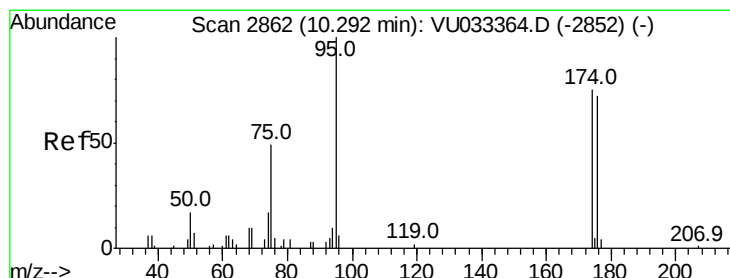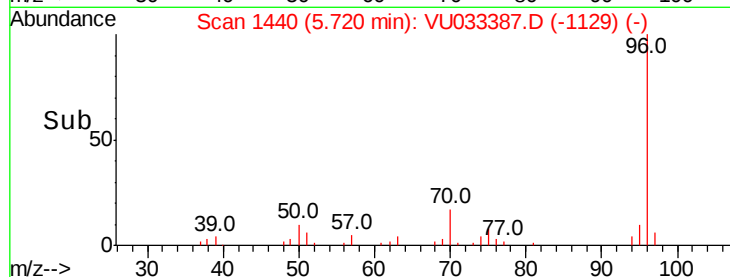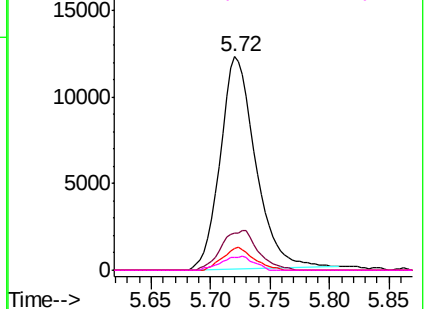

#57

4-Bromofluorobenzene

Concen: 0.798 ug/l

RT: 10.30 min Scan# 2863

Delta R.T. 0.00 min

Lab File: VU033387.D

Acq: 24 Jul 2019 11:42


Tgt Ion: 95 Resp: 7915

Ion Ratio Lower Upper

95 100

174 79.6 58.8 88.2



176 73.7 54.4 81.6

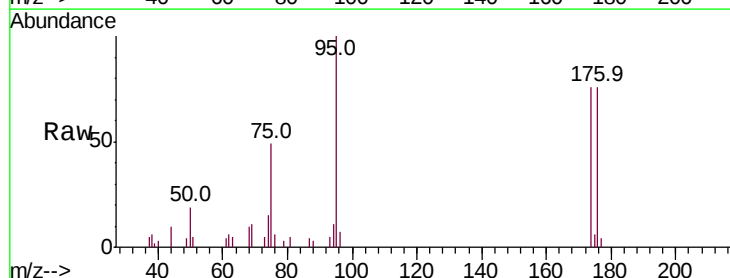


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

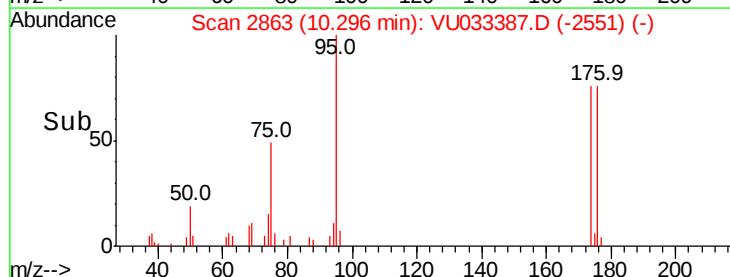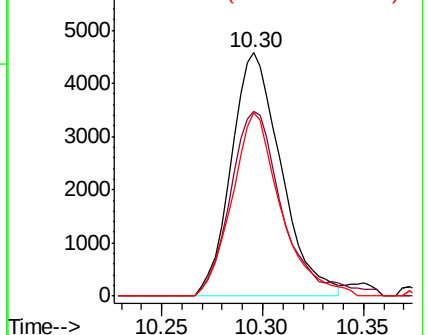

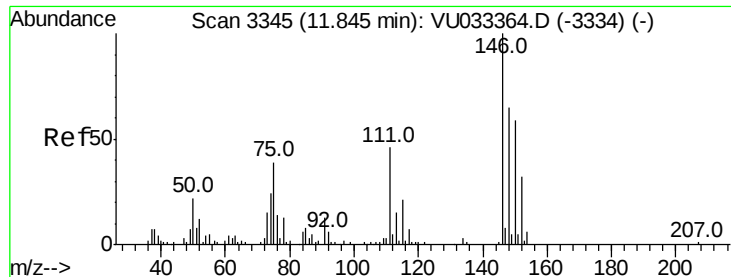

#68

1,2-Dichlorobenzene-d4

Concen: 0.817 ug/l

RT: 11.85 min Scan# 3345

Delta R.T. -0.00 min

Lab File: VU033387.D

Acq: 24 Jul 2019 11:42

Instrument :

MSVOA_U

ClientSampleId :

VU0724WBL01

Tot Ion:152 Resp: 8358

Ion Ratio Lower Upper

152 100

115 65.9 0.0 123.2

150 162.7 0.0 648.4

