


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072419\
 Data File : VU033385.D
 Acq On : 24 Jul 2019 10:23
 Operator : JC/SP
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072219DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Wed Jul 24 03:53:19 2019

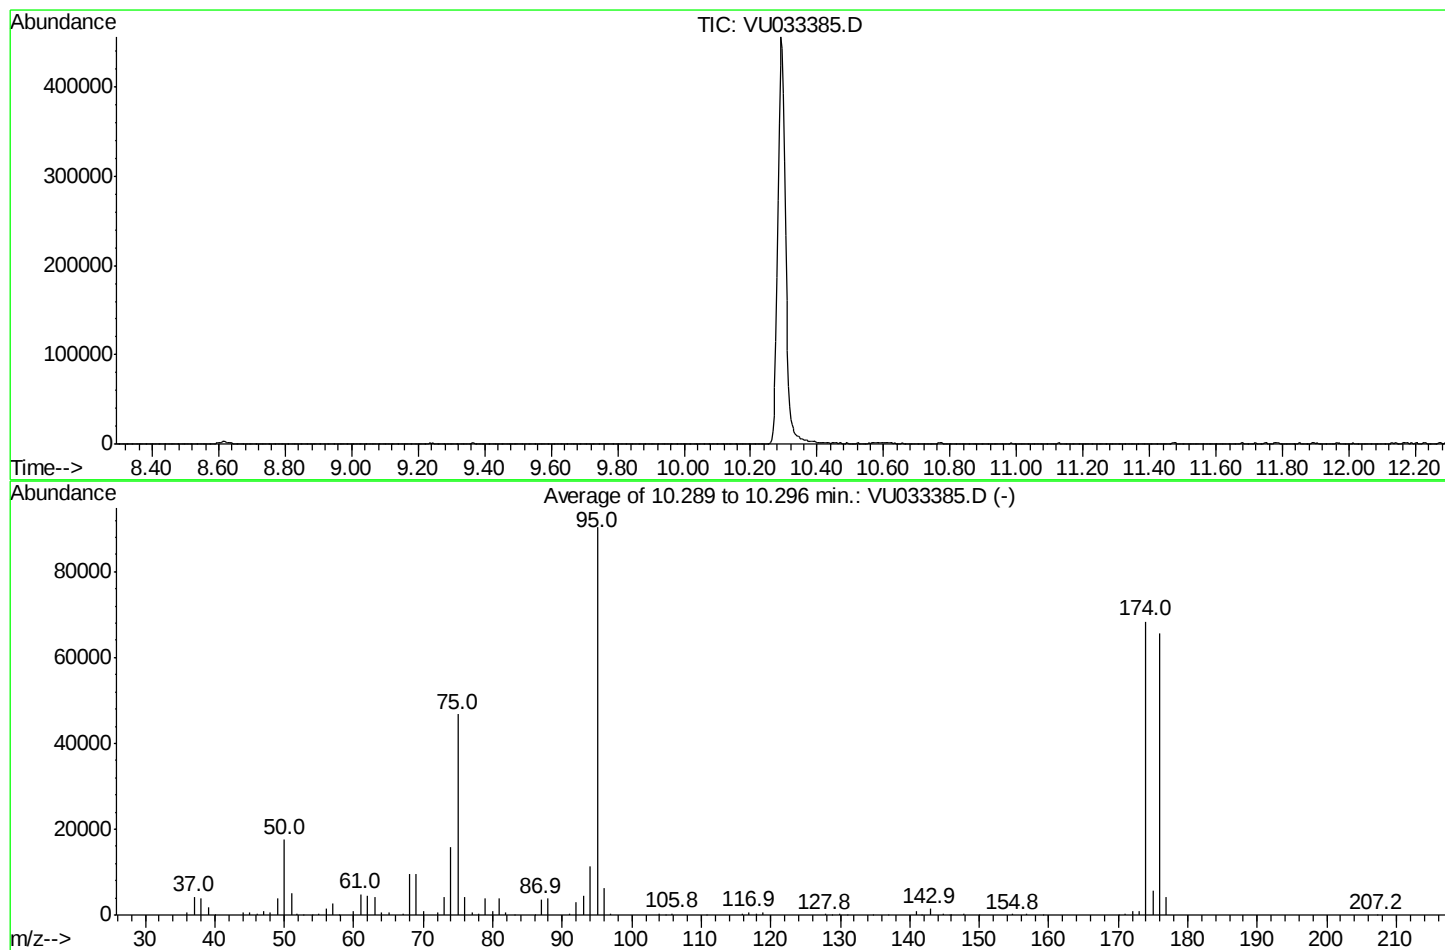

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	17485	PASS
75	95	30	60	51.8	46778	PASS
95	95	100	100	100.0	90344	PASS
96	95	5	9	6.8	6181	PASS
173	174	0.00	2	1.4	960	PASS
174	95	50	100	75.7	68381	PASS
175	174	5	9	8.5	5819	PASS
176	174	95	101	96.2	65776	PASS
177	176	5	9	6.5	4302	PASS