


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072420\
Data File : VU039655.D
Acq On : 24 Jul 2020 09:11
Operator : SY/MD
Sample : BFB52
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072320WMA.M
Title : VOC Analysis
Last Update : Mon Jul 27 06:24:08 2020

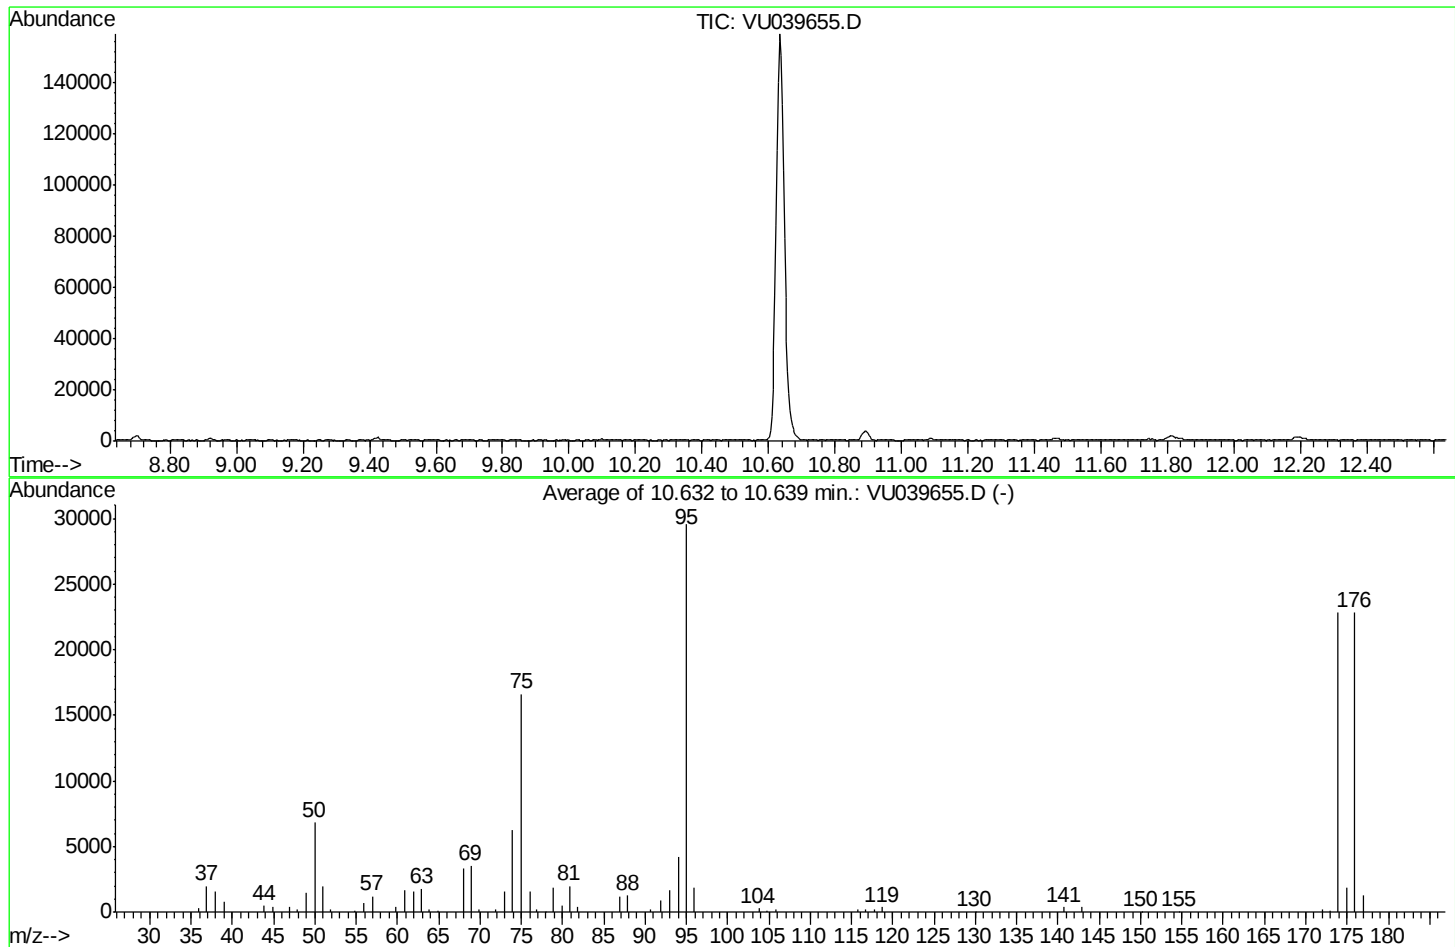

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	6808	PASS
75	95	30	80	56.3	16640	PASS
95	95	100	100	100.0	29560	PASS
96	95	5	9	6.1	1816	PASS
173	174	0.00	2	0.4	95	PASS
174	95	50	120	77.2	22810	PASS
175	174	5	9	8.0	1826	PASS
176	174	95	101	100.0	22818	PASS
177	176	5	9	5.7	1311	PASS

Scan 2877 (10.590 min): VU039655.D
BFB52

m/z	Abundance
39.80	143.0
43.90	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.90	319.0
36.90	2016.0
38.00	1610.0
39.00	892.0
39.90	139.0
43.90	684.0
44.90	339.0
47.00	418.0
47.90	247.0
49.00	1520.0
50.00	6841.0
50.90	2015.0
51.90	174.0
54.80	123.0
55.90	716.0
57.00	1268.0
59.90	371.0
60.90	1678.0
61.90	1475.0
62.90	1855.0
63.90	148.0
64.90	126.0
68.00	3274.0
68.90	3894.0
69.80	304.0
71.80	144.0
72.90	1565.0
74.00	6271.0
75.00	17104.0
76.00	1575.0
76.80	205.0
78.00	136.0
78.80	1821.0
79.90	526.0
80.80	1983.0
81.80	441.0
86.90	1244.0
87.90	1344.0
90.70	170.0
92.00	881.0
92.90	1673.0
94.00	4229.0
95.00	29744.0
95.90	1961.0
103.80	219.0
104.70	110.0
105.90	234.0
115.80	150.0
116.70	262.0
117.70	219.0
118.80	375.0
140.80	398.0
142.80	406.0
150.10	127.0
154.70	100.0
171.90	217.0
173.90	22496.0
175.00	1821.0
175.90	21912.0
176.90	1297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.80	277.0
36.90	2099.0
38.00	1639.0
39.00	822.0
39.90	143.0
43.90	671.0
44.90	383.0
47.00	378.0
47.80	245.0
48.90	1490.0
50.00	6989.0
50.90	2058.0
51.90	170.0
54.80	106.0
56.00	678.0
57.00	1223.0
59.90	381.0
60.90	1716.0
61.90	1621.0
63.00	1830.0
63.80	186.0
64.80	124.0
67.90	3420.0
68.90	3636.0
69.80	226.0
71.90	182.0
72.90	1564.0
74.00	6404.0
75.00	17120.0
76.00	1650.0
76.80	173.0
78.80	1838.0
79.90	537.0
80.90	2031.0
81.80	421.0
86.90	1224.0
87.90	1309.0
90.70	192.0
92.00	917.0
92.90	1647.0
94.00	4417.0
95.00	30296.0
95.90	1830.0
103.80	258.0
104.70	102.0
105.90	236.0
115.80	177.0
116.70	229.0
117.70	206.0
118.80	396.0
140.80	388.0
142.90	353.0
172.00	231.0
173.90	23296.0
175.00	1868.0
175.90	23544.0
176.90	1365.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.80	284.0
36.90	1868.0
38.00	1588.0
38.90	698.0
39.80	121.0
43.90	627.0
44.90	356.0
47.00	252.0
47.70	245.0
48.90	1449.0
49.90	6595.0
50.90	1829.0
51.90	141.0
56.00	646.0
57.00	1081.0
59.80	387.0
60.90	1609.0
61.90	1709.0
63.00	1630.0
63.80	194.0
64.80	119.0
67.90	3255.0
68.90	3163.0
69.80	193.0
72.00	228.0
72.90	1529.0
73.90	5988.0
75.00	15696.0
76.00	1557.0
76.90	166.0
78.90	1777.0
79.90	507.0
80.90	1866.0
81.90	365.0
86.90	1113.0
87.90	1135.0
90.70	174.0
91.90	877.0
92.90	1555.0
94.00	4097.0
95.00	28640.0
96.00	1659.0
103.80	270.0
105.90	209.0
115.70	183.0
116.80	172.0
117.80	170.0
118.70	341.0
130.00	104.0
140.70	350.0
142.90	341.0
172.00	218.0
173.00	286.0
173.90	22640.0
174.90	1791.0
175.90	23000.0
176.90	1273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52