

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072423\
 Data File : VU054850.D
 Acq On : 24 Jul 2023 10:58
 Operator : MD/SY
 Sample : VU0724WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0724WBL01

Quant Time: Jul 25 02:12:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072123DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Mon Jul 24 09:59:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	26685	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	7421	0.921	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	
68) 1,2-Dichlorobenzene-d4	12.196	152	9071	0.972	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072423\
Data File : VU054850.D
Acq On : 24 Jul 2023 10:58
Operator : MD/SY
Sample : VU0724WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0724WBL01

Quant Time: Jul 25 02:12:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072123DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Mon Jul 24 09:59:15 2023
Response via : Initial Calibration




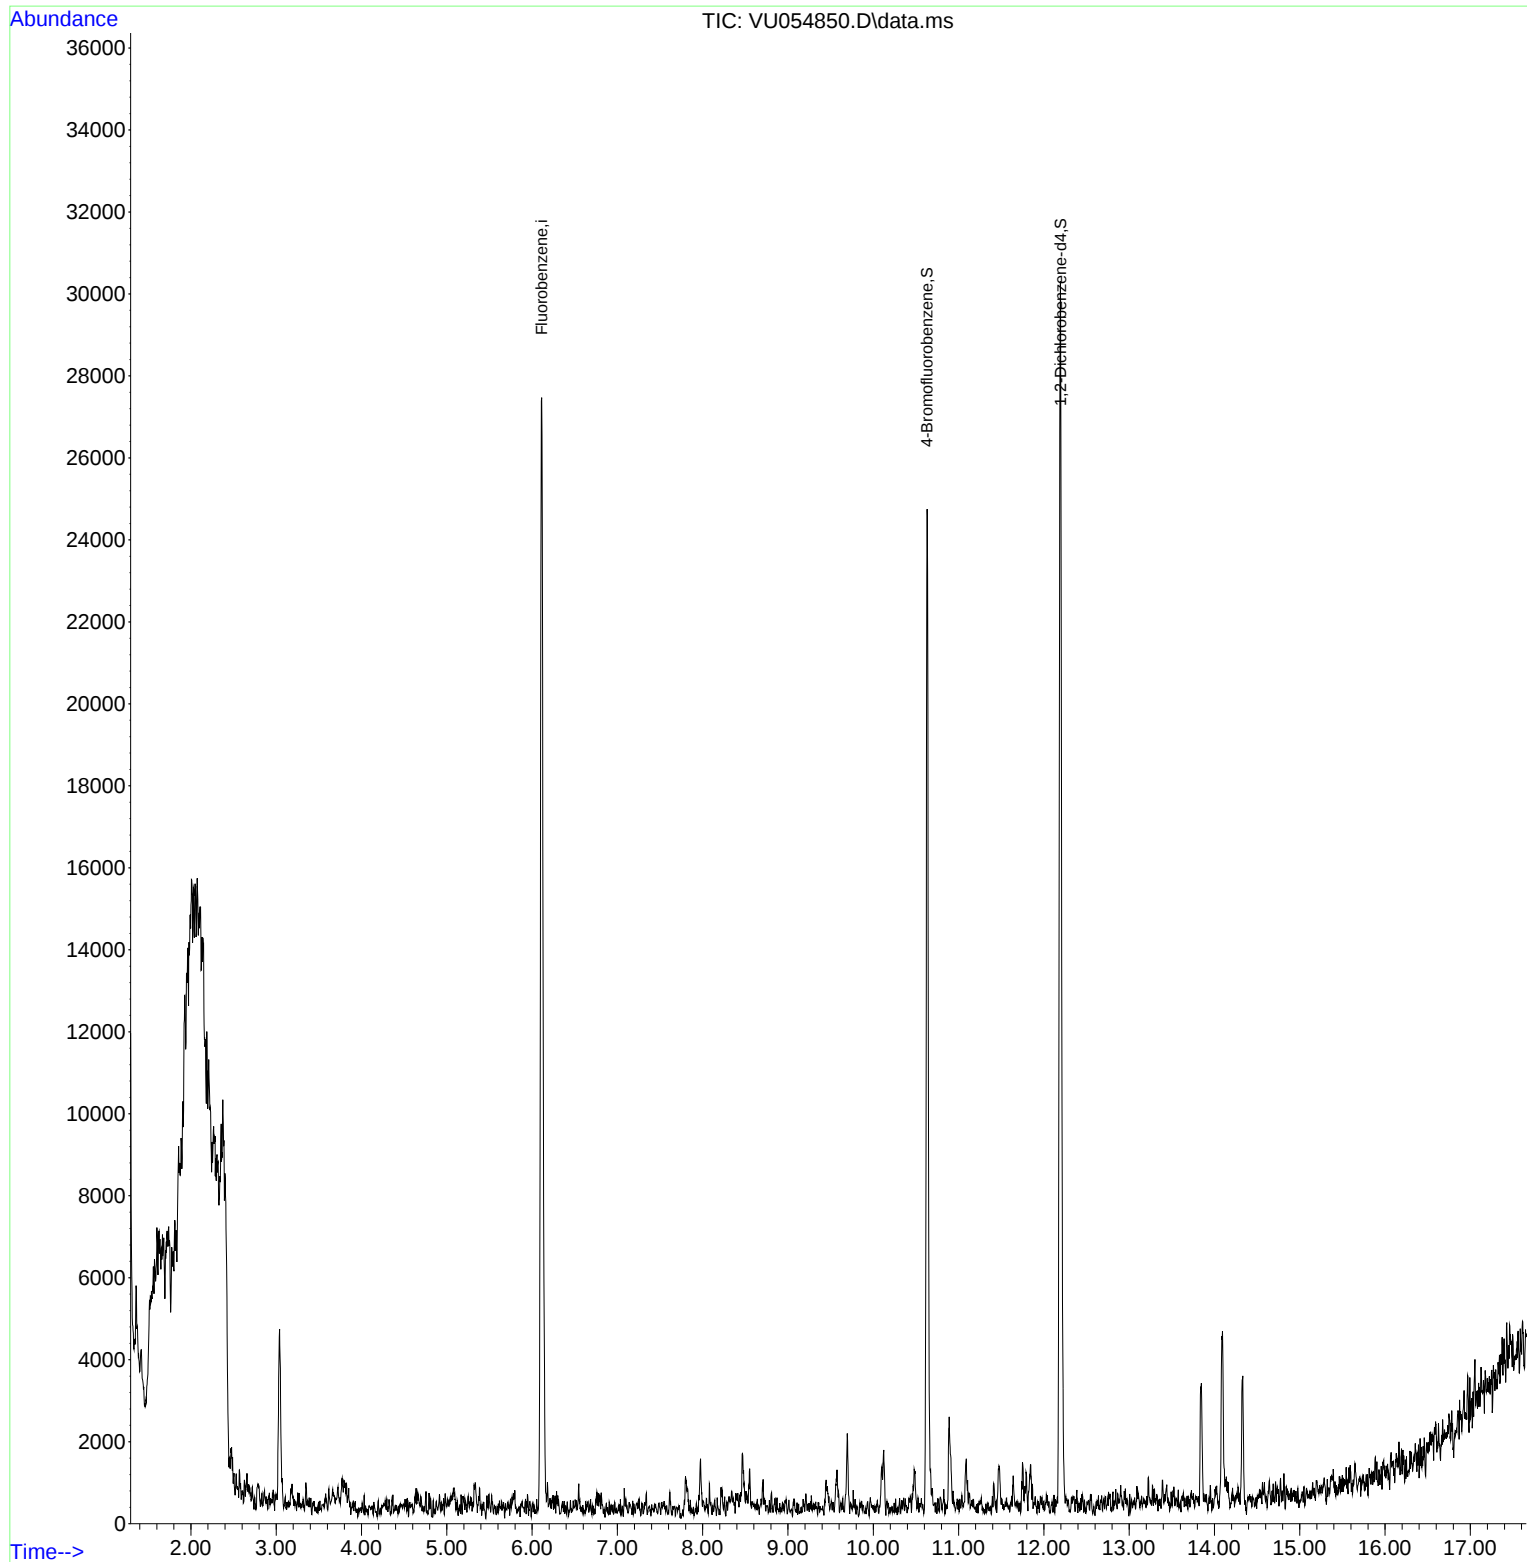


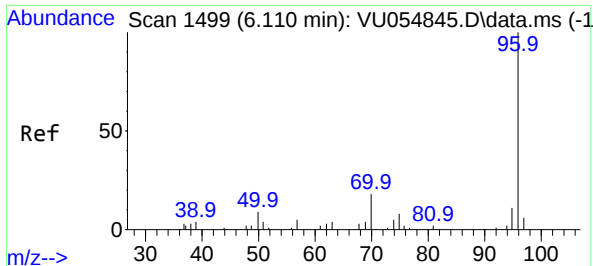

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1499
Delta R.T. 0.003 min
Lab File: VU054850.D
Acq: 24 Jul 2023 10:58




Instrument :
MSVOA_U
ClientSampleId :
VU0724WBL01


Tgt Ion: 96	Resp: 26685
Ion Ratio	Lower Upper
96 100	
70 19.1	14.0 21.0
95 9.3	8.7 13.1
97 3.6	0.0 0.0

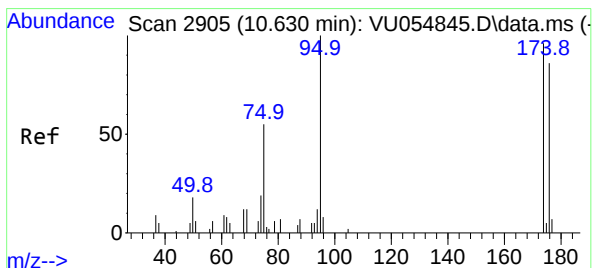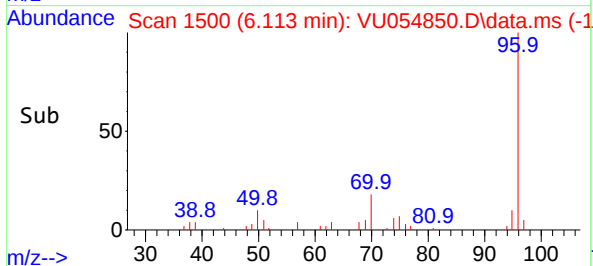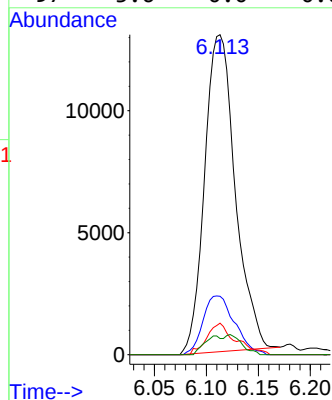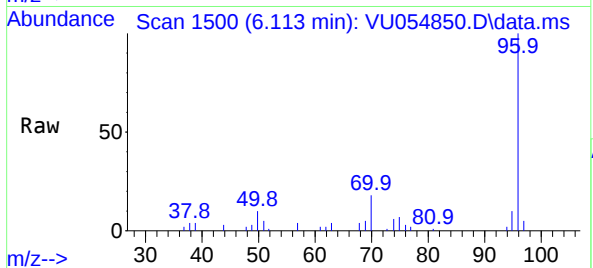

#57
4-Bromofluorobenzene
Concen: 0.921 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.000 min
Lab File: VU054850.D
Acq: 24 Jul 2023 10:58


Tgt Ion: 95	Resp: 7421
Ion Ratio	Lower Upper
95 100	
174 95.4	79.3 118.9
176 95.6	71.5 107.3

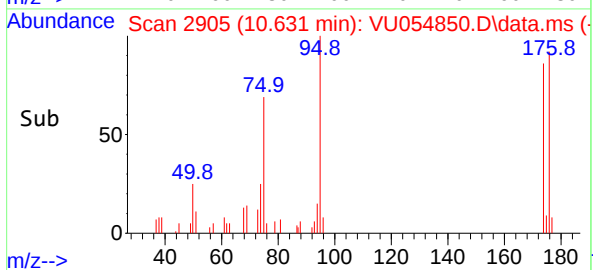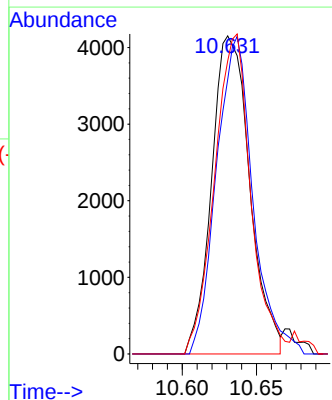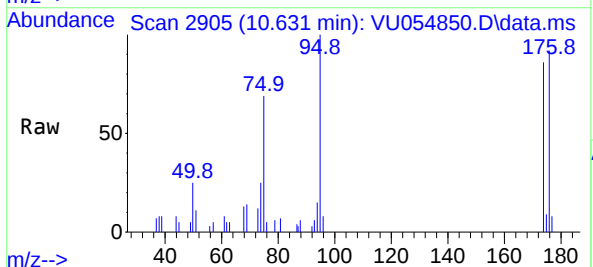

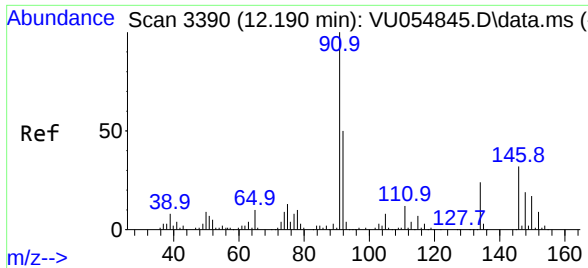

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.972 ug/l
 RT: 12.196 min Scan# 31
 Delta R.T. 0.007 min
 Lab File: VU054850.D
 Acq: 24 Jul 2023 10:58

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0724WBL01

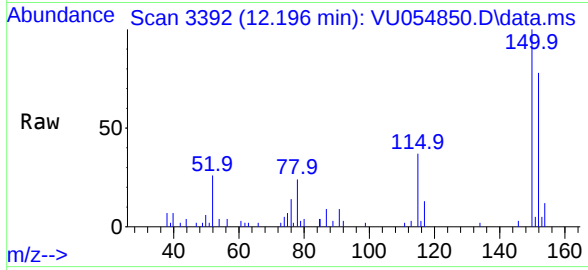

Tgt Ion:	152	Resp:	9071
Ion Ratio	Lower	Upper	
152	100		
115	55.5	0.0	234.8
150	144.5	0.0	598.2

