

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072423\
 Data File : VU054863.D
 Acq On : 24 Jul 2023 16:41
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Jul 25 02:15:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072123DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Mon Jul 24 09:59:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.113	96	26680	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	7823	0.971	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	8451	0.906	ug/l	0.00
Spiked Amount 1.000			Recovery	=	91.000%	
Target Compounds						
15) Methylene Chloride	3.039	84	10945	1.102	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072423\
Data File : VU054863.D
Acq On : 24 Jul 2023 16:41
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Jul 25 02:15:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072123DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Mon Jul 24 09:59:15 2023
Response via : Initial Calibration




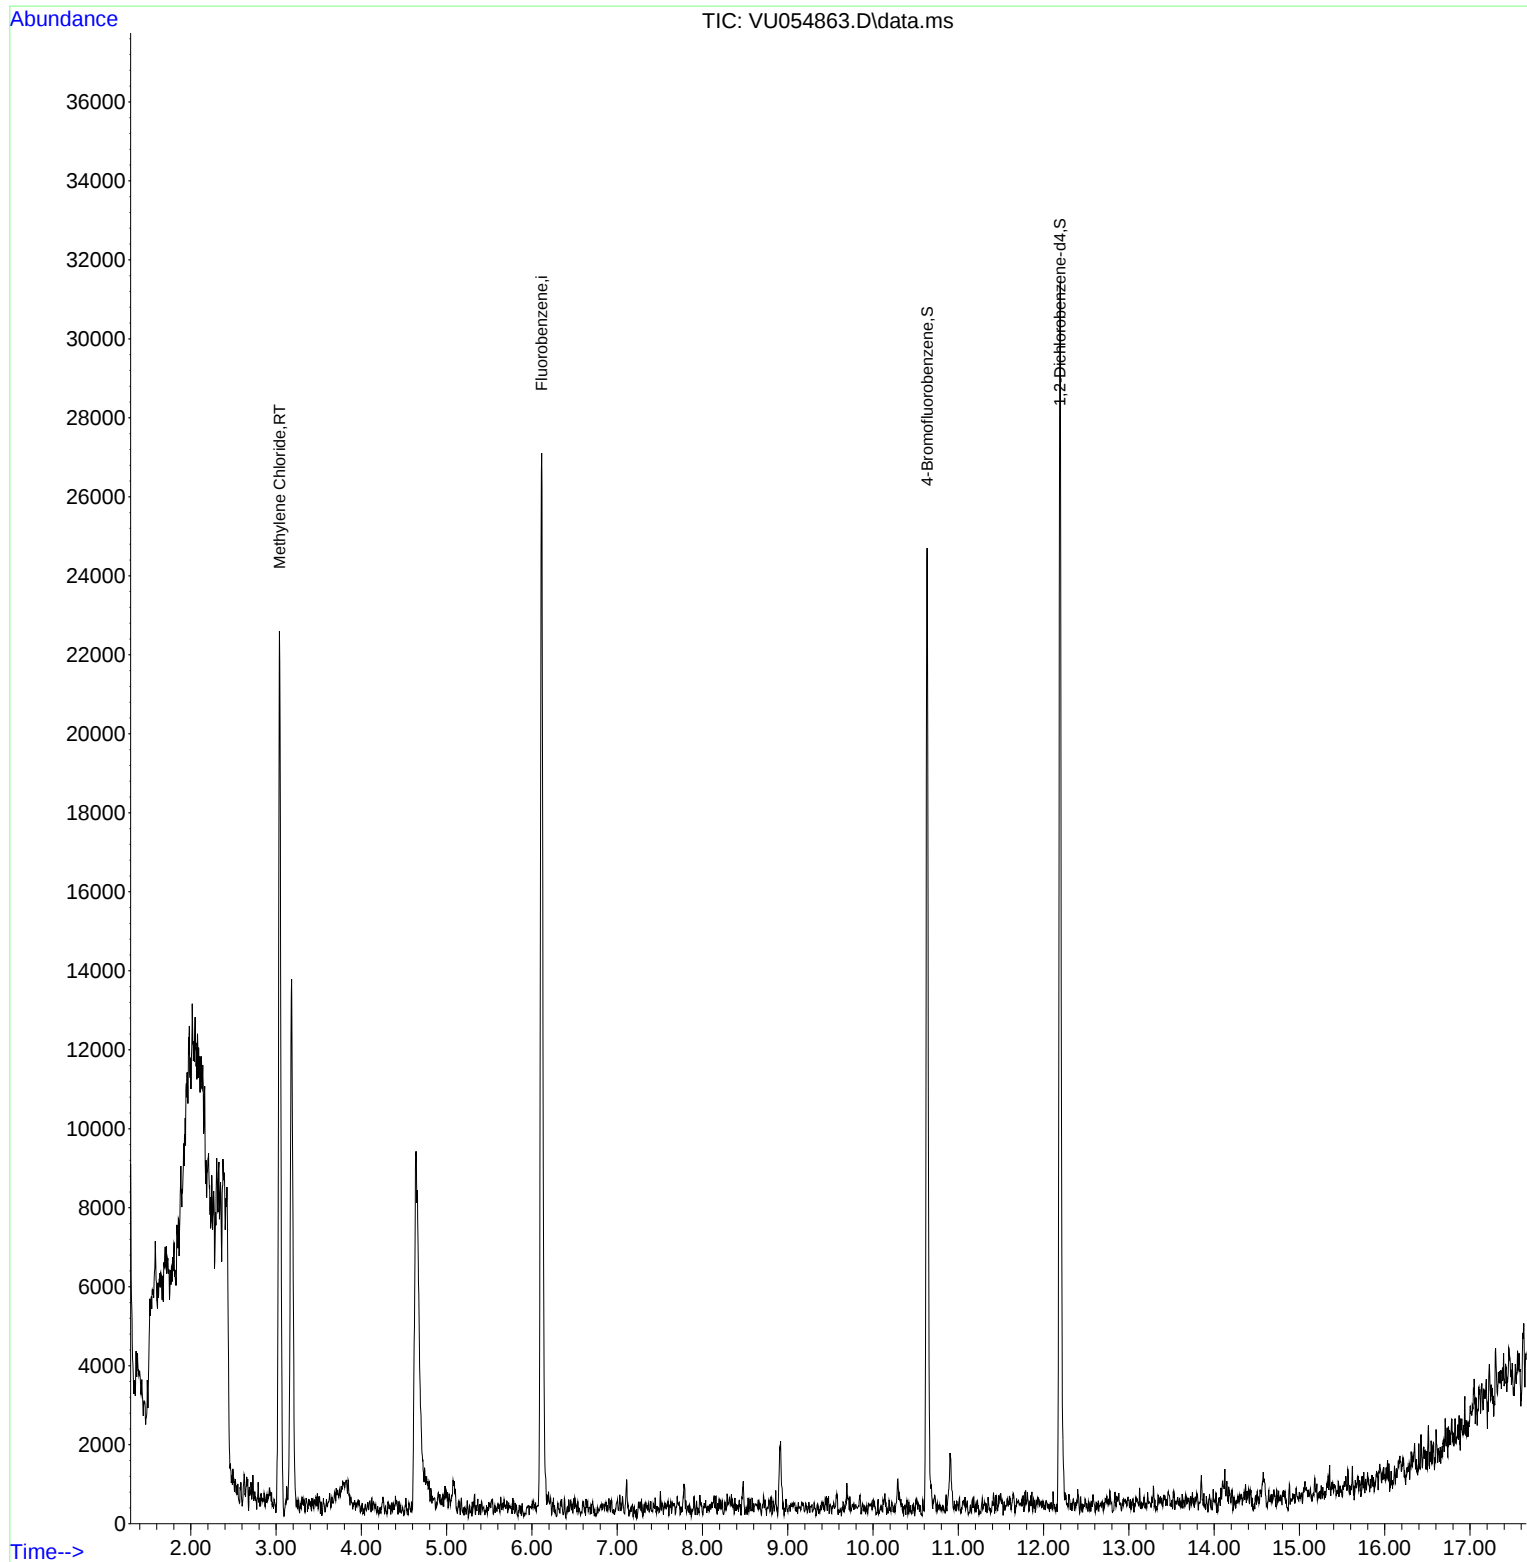


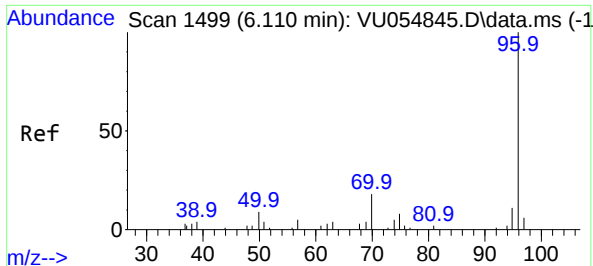

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU054863.D
Acq: 24 Jul 2023 16:41




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion:	96	Resp:	26680
Ion	Ratio	Lower	Upper
96	100		
70	17.7	14.0	21.0
95	7.4	8.7	13.1#
97	5.6	0.0	0.0#

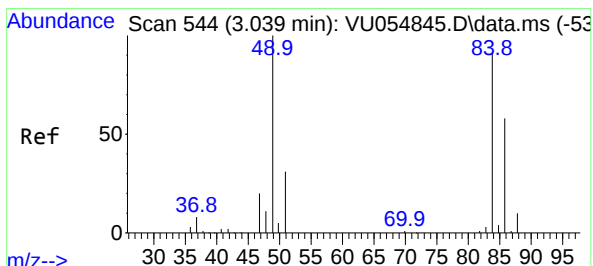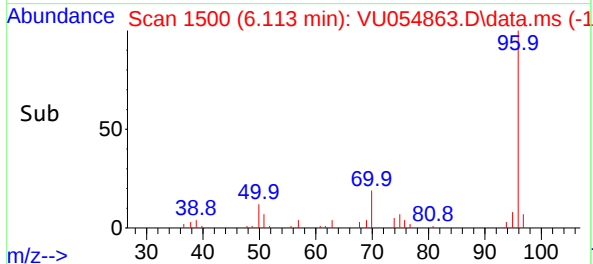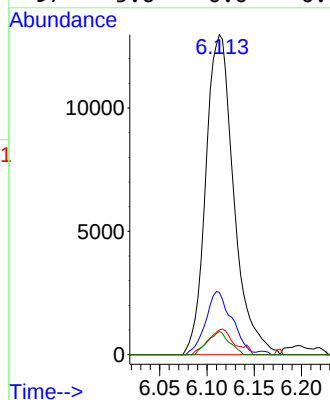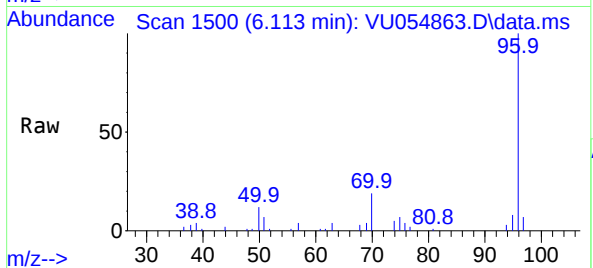

#15
Methylene Chloride
Concen: 1.102 ug/l
RT: 3.039 min Scan# 544
Delta R.T. 0.000 min
Lab File: VU054863.D
Acq: 24 Jul 2023 16:41

Tgt Ion:	84	Resp:	10945
Ion	Ratio	Lower	Upper
84	100		
49	109.5	87.8	131.6
51	30.8	0.0	68.2
86	62.8	51.0	76.4


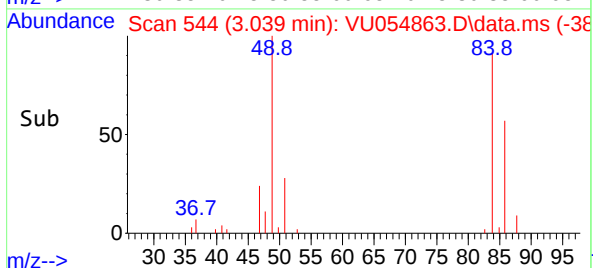
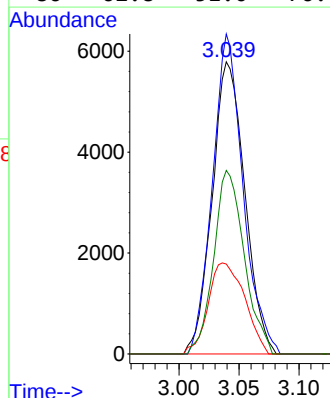
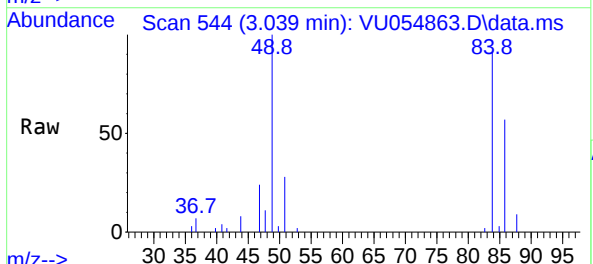


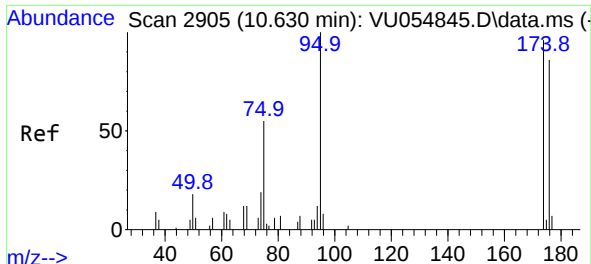

#57
 4-Bromofluorobenzene
 Concen: 0.971 ug/l
 RT: 10.634 min Scan# 2905
 Delta R.T. 0.003 min
 Lab File: VU054863.D
 Acq: 24 Jul 2023 16:41

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Tgt Ion: 95 Resp: 7823
 Ion Ratio Lower Upper
 95 100
 174 91.5 79.3 118.9
 176 94.6 71.5 107.3

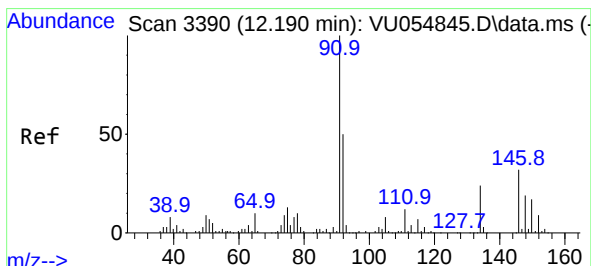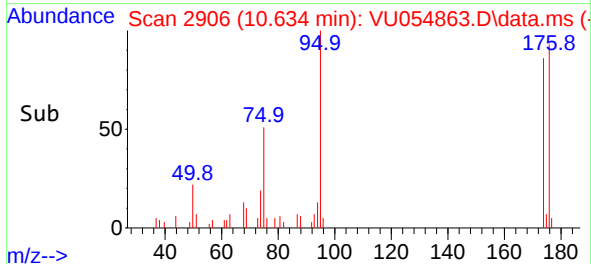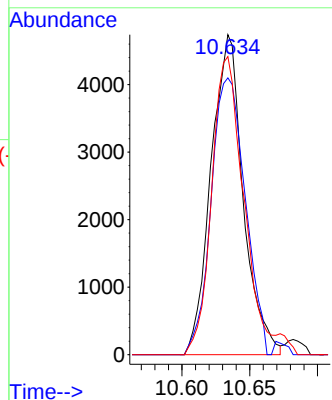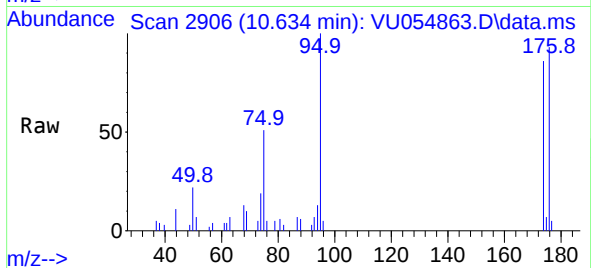

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.906 ug/l
 RT: 12.190 min Scan# 3390
 Delta R.T. 0.000 min
 Lab File: VU054863.D
 Acq: 24 Jul 2023 16:41

Tgt Ion: 152 Resp: 8451
 Ion Ratio Lower Upper
 152 100
 115 58.2 0.0 234.8
 150 161.1 0.0 598.2

