


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072423\
Data File : VU054848.D
Acq On : 24 Jul 2023 08:58
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072123DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Mon Jul 24 09:59:15 2023

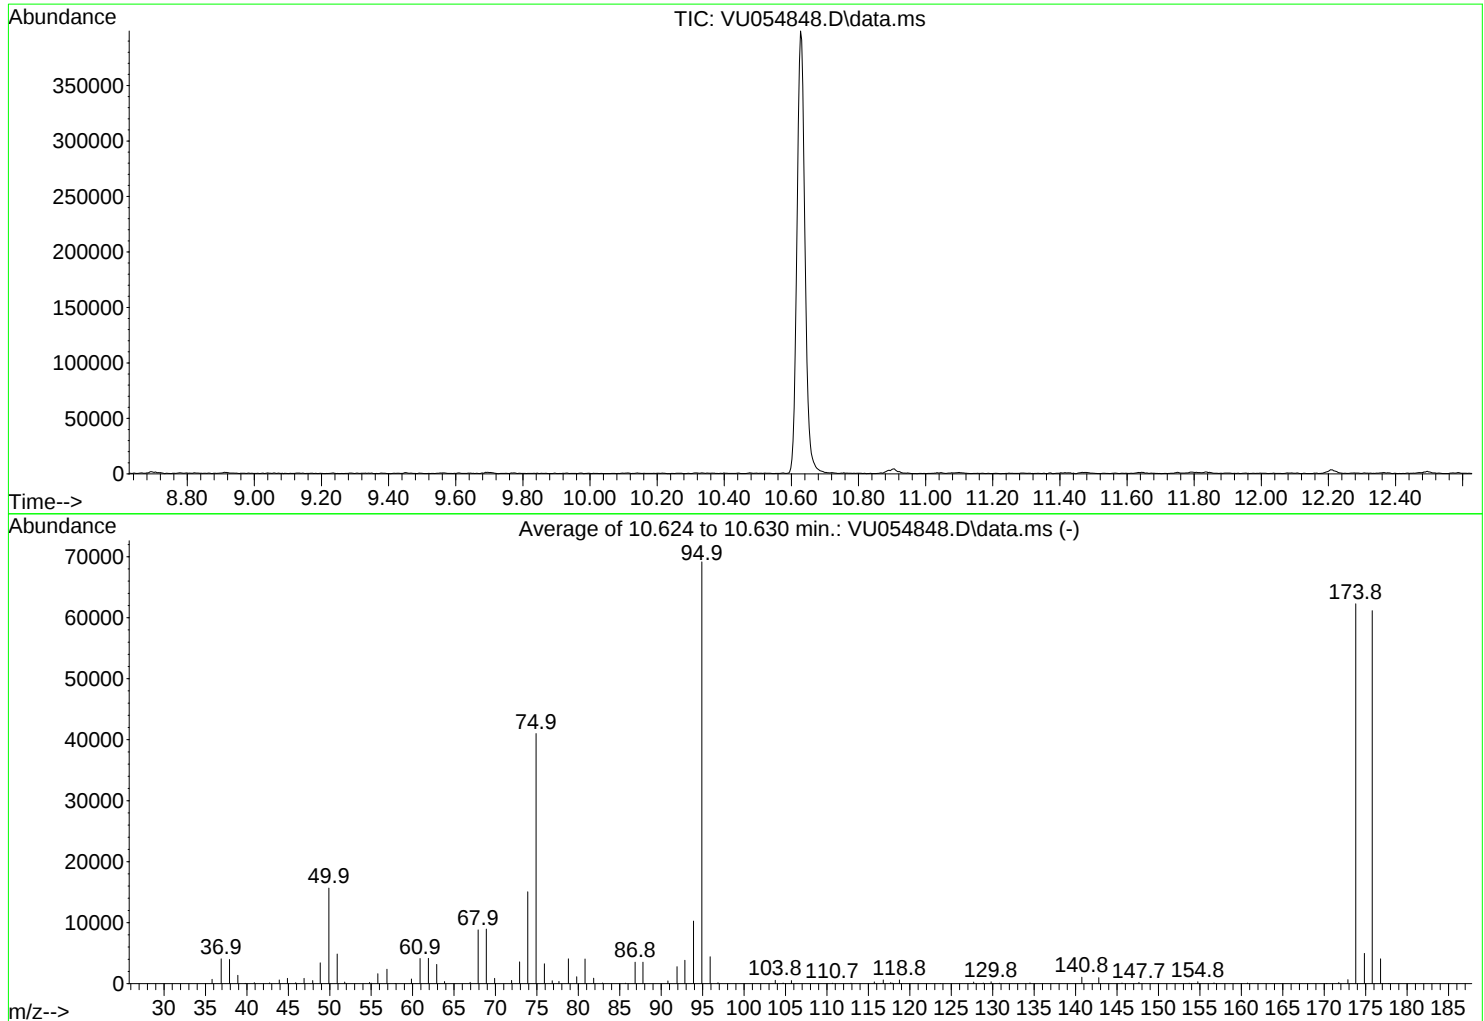

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	15676	PASS
75	95	30	60	59.3	41000	PASS
95	95	100	100	100.0	69163	PASS
96	95	5	9	6.4	4412	PASS
173	174	0.00	2	1.1	654	PASS
174	95	50	100	90.0	62277	PASS
175	174	5	9	8.0	4973	PASS
176	174	95	101	98.2	61144	PASS
177	176	5	9	6.6	4063	PASS