


Iodomethane

Response Ratio

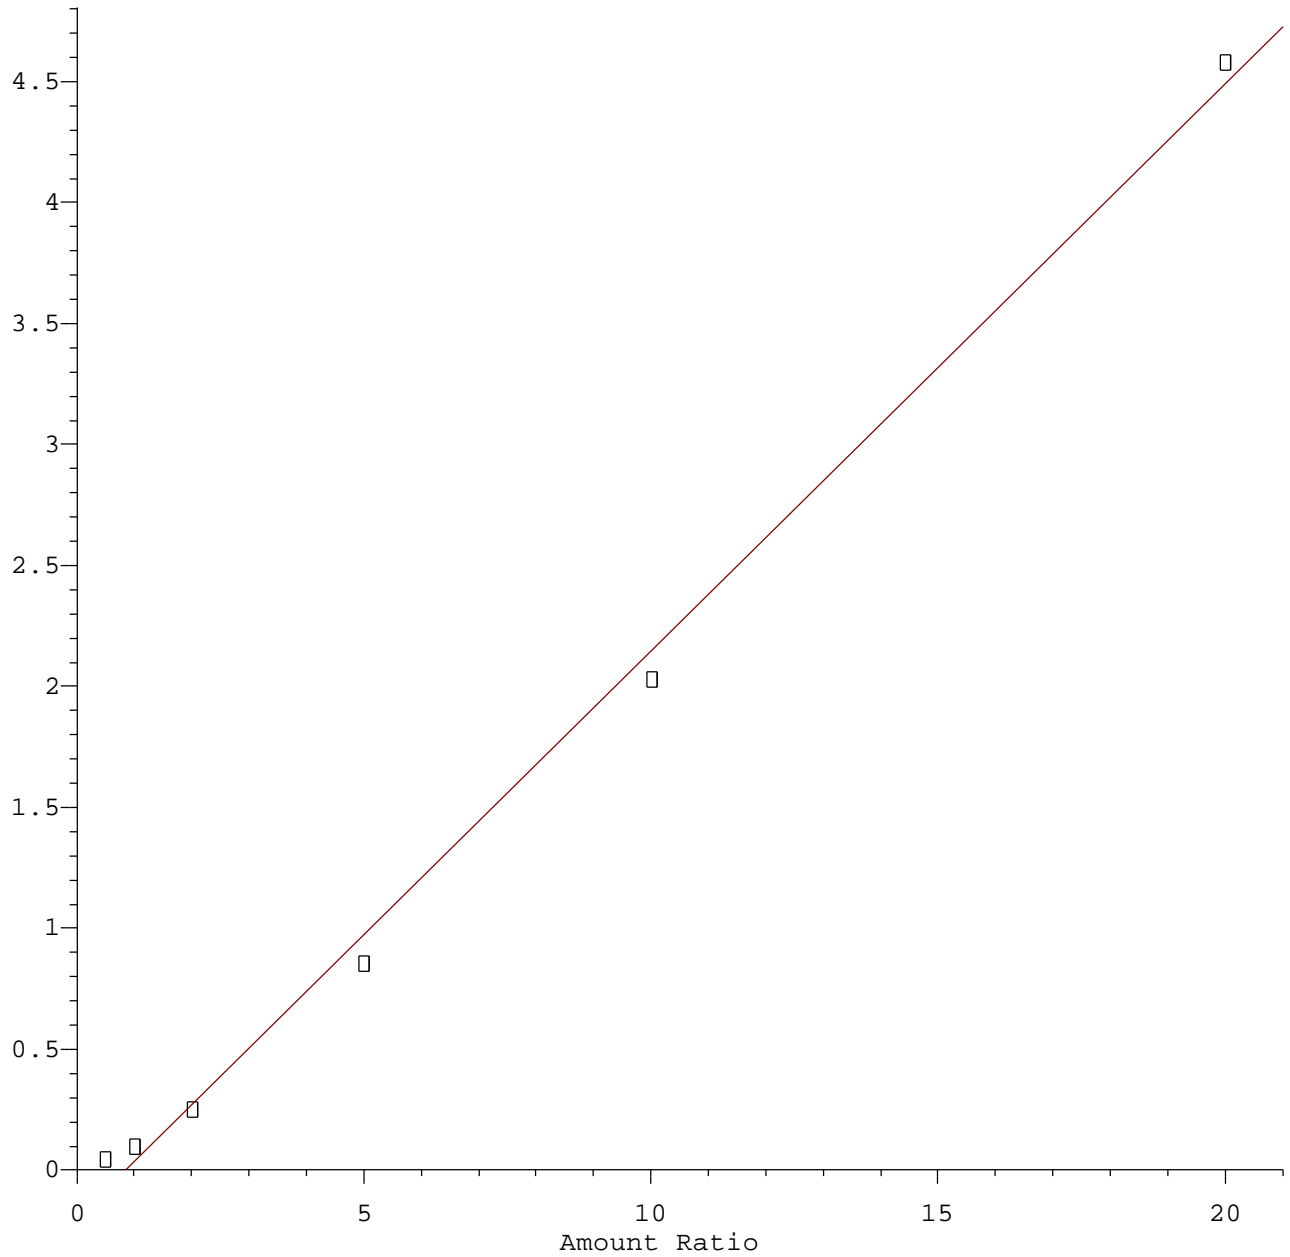


Resp Ratio = 2.34e-001 \* Amt - 1.96e-001  
Coef of Det (r^2) = 0.996    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\524U072518DW.M  
Calibration Table Last Updated: Fri Jul 27 15:10:58 2018

t-1,4-Dichloro-2-butene

Response Ratio

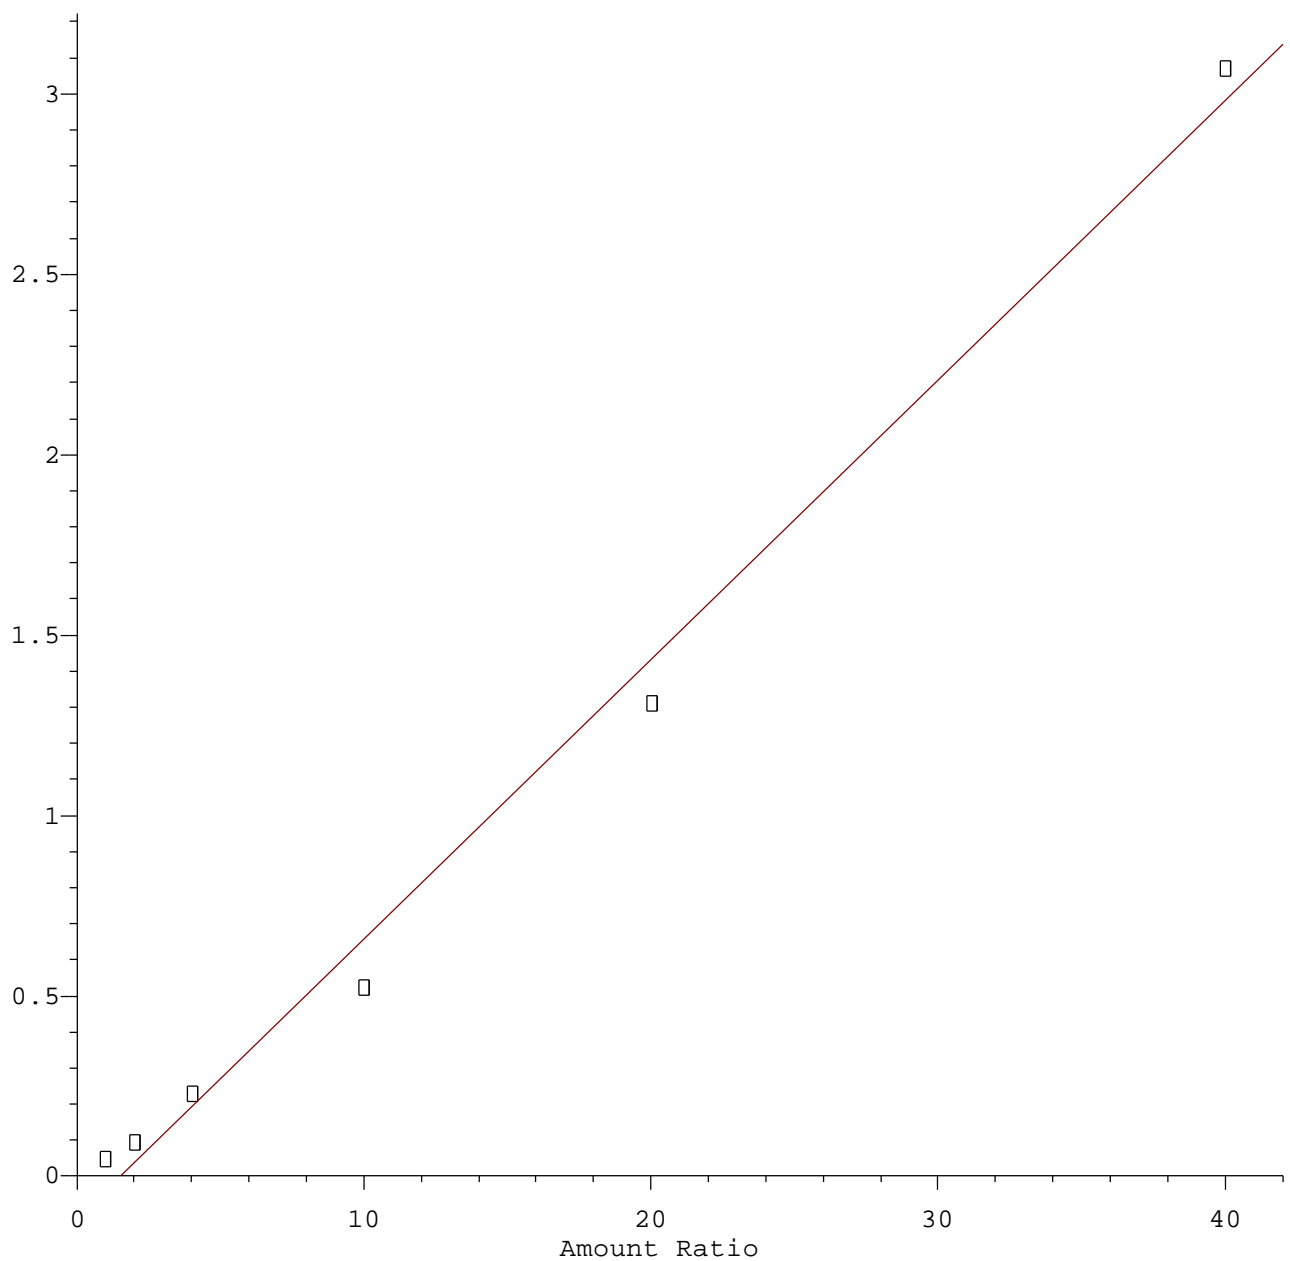

Resp Ratio =  $7.74e-002 * Amt - 1.16e-001$   
Coef of Det ( $r^2$ ) = 0.992 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\524U072518DW.M  
Calibration Table Last Updated: Fri Jul 27 15:10:58 2018